


pulse oximetry

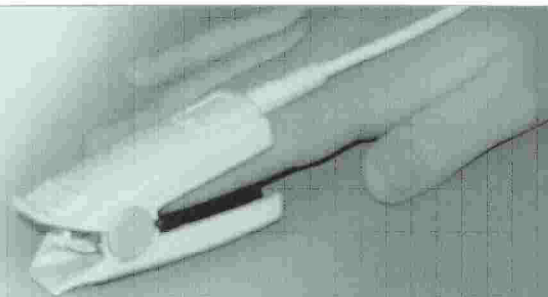

800 Series SpO₂ Sensors

- For use in continuous monitoring of oxygen saturation and pulse rate.
- Sensors compatible for use with a wide range of manufacturers' pulse oximeters.
- Sensors specifically compatible (not generic) to OEM sensors.
- Quality proven durable design.
- Cost-effective.


A wide range of extension and adapter cables are available for use with 800 Series sensors. Adapter cables enable use of 800 Series sensors on an extended range of manufacturers' pulse oximeters and patient monitors.

Also available:

- Pulse oximetry sensor and cable repair services.
- Service kits.
- Viamed DL3000 pulse oximetry simulator.
- Viamed VG900 sensor test unit.
- OEM sensors and cables.
- Additional series of compatible sensors and cables.

Range includes:

- Reusable finger sensors
- Reusable multi-site 'Y' sensors
- Extension cables
- Adapter cables

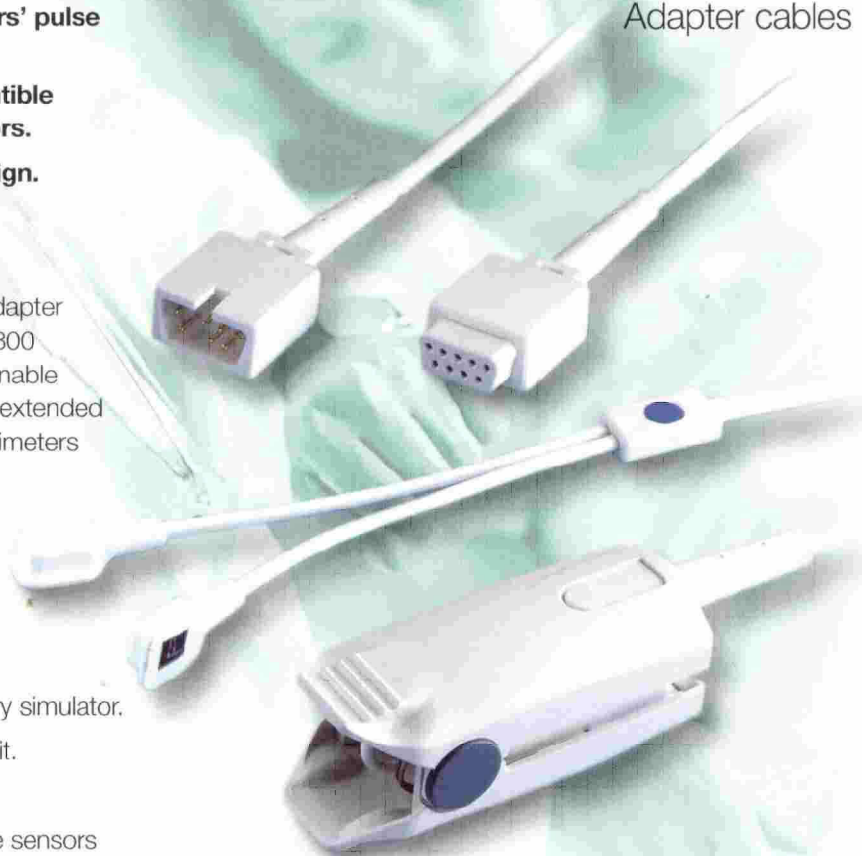

 **VIAMED**

Viamed 800 Series

pulse oximetry finger sensors and multi-site 'Y' sensors.

Part number	Finger sensor	Part number	'Y' sensor	Oximeter manufacturer	Cable length (m)	Connector type	Connector contacts	Connector gender
0018520	P852RA			Nihon Kohden	3.00	Nihon Kohden	10	M
0018530	P853RA			Odham Bruker	3.00	Odham	12	M
0018540	P854RA			Medlab, Comdek	3.00	Redel, 2 key ways	7	M
0018550	P855RA			BCI	3.00	Redel, 1 key way	7	M
0018560	P856RA	0018562	P856YA	Nellcor	0.90	D	9	M
0018570	P857RA	0018572	P857YA	Spacelabs	3.00	Hypertronics	12	M
0018580	P858RA	0018582	P858YA	Nellcor	3.65	D	9	M
0018590	P859RA	0018592	P859YA	Pace Tech	3.65	Switchcraft	5	F
0018600	P860RA	0018602	P860YA	Simed, Baxter	3.65	Hypertronics	9	M
0018610	P861RA	0018612	P861YA	BCI	0.90	D	9	M
0018620	P862RA			Criticare	3.00	Lemo	5	M
0018630	P863RA			Datascope	0.90	D	9	M
0018640	P864RA	0018642	P864YA	Datascope	3.65	DIN	8	M
0018650	P865RA			Sensormedics	0.90	Compu-shield	6	M
0018660	P866RA	0018662	P866YA	Simed, Baxter	3.65	Hypertronics	9	M
0018670	P867RA	0018672	P867YA	Ohmeda	3.65	Hypertronics	9	M
0018680	P868RA			Criticare	0.90	D, right angled	9	M
0018690	P869RA	0018692	P869YA	Criticare	0.90	D	9	M
0018700	P870RA			Criticare	3.00	D, right angled	9	M
0018710	P871RA	0018712	P871YA	Nonin	0.90	D	9	M
0018720	P872RA			Datex	3.65	DPK1	10	F
0018730	P873RA	0018732	P873YA	Datex	0.90	D	9	M
0018740	P874RA			Palco	0.90	Sub min	6	M
0018750	P875RA	0018752	P875YA	Novamatrix	3.00	Hypertronics	7	M
0018760	P876RA	0018762	P876YA	Novamatrix	3.00	Hypertronics	7	M
0018770	P877RA			Critikon	0.90	D	9	M
0018780	P878RA	0018782	P878YA	Invivo	3.00	Lemo	7	M
0018790	P879RA			Artema	3.65	SPK1-A	12	M
0018800	P880RA			Nonin	2.40	D	9	M
0018850	P885RA			Novamatrix	0.90	D	9	M
0018860	P886RA	0018862	P886YA	Kontron	3.65	DPK1	12	M
0018870	P887RA	0018872	P887YA	Spacelabs	3.00	Hypertronics	12	M
0018880	P888RA	0018882	P888YA	S & W	3.65	SPK1-O	10	F
0018890	P889RA			Criticare	3.00	D	9	M
0018900	P890RA			Critikon/Sensormedics	3.00	Thorkom	12	F
0018910	P891RA			Critikon	3.00	Lemo	7	M
0018920	P892RA	0018922	P892YA	Marquette	3.00	Marquette	11	M
0018960	P896RA	0018962	P896YA	S&W	3.65	SPK1-N	10	F

Accessories

0021002	P100E	Ear clip for use with multi-site 'Y' sensor.
0021012	6554	Probe wrap – adult or paediatric finger, infant toe, neonatal foot. For use with multi-site 'Y' sensor.
0021013	6554	Probe wrap – adult or paediatric finger, infant toe, neonatal foot. For use with multi-site 'Y' sensor. Pack of 12.

Contact Viamed regarding compatibility and cross reference data.

All 800 series pulse oximetry sensors and cables are latex free.

Specifications subject to change.



Distributed by:



Viamed Limited · 15 Station Road · Cross Hills
 Keighley · West Yorkshire · BD20 7DT · United Kingdom
 Tel: +44 (0)1535 634542/636757 Fax: +44 (0)1535 635582
 Email: info@viamed.co.uk Website: www.viamed.co.uk



BS EN ISO 9001
 BS EN 46001
 BS EN ISO 13485