

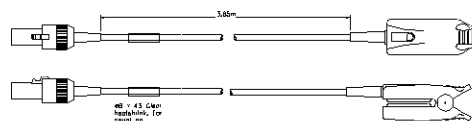


Hypertronics Male 9 Pin

Finger Probe

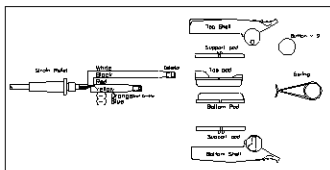


9P = 45 Ohm
hypertronics, for
series 102




Hypertronics Male 9 Pin

Finger Probe

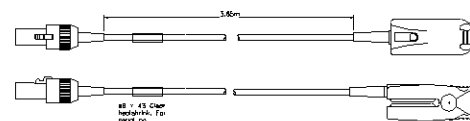

9P = 45 Ohm
hypertronics, for
series 102


Hypertronics male 9 pin




9P = 45 Ohm
hypertronics, for
series 102

Hypertronics Male 9 Pin


Finger Probe



Enlarged front view

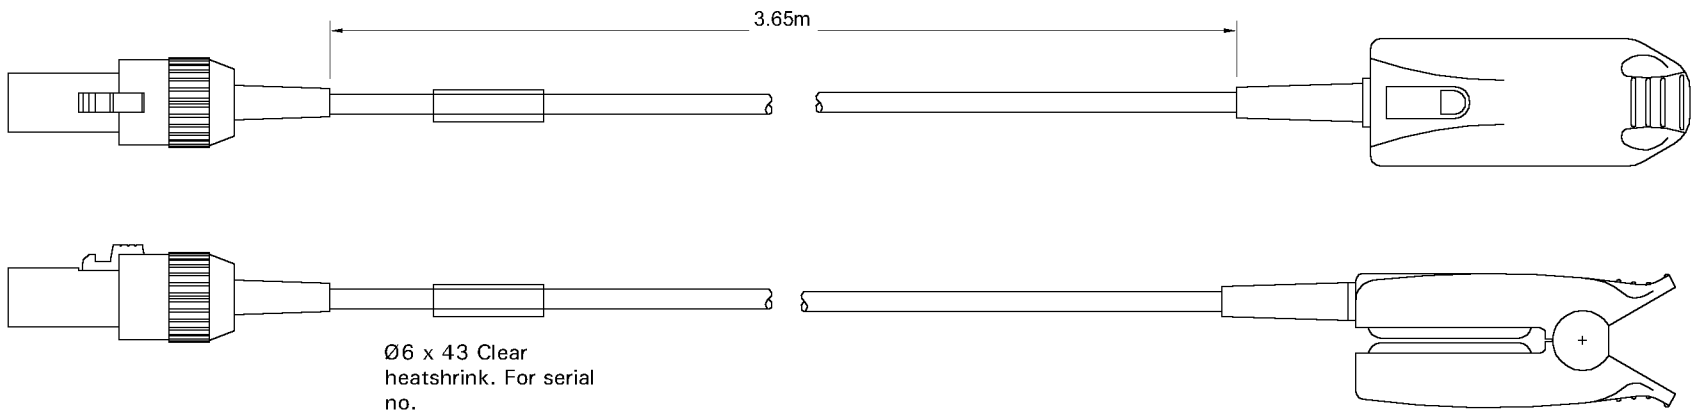

Hypertronics male 9 pin

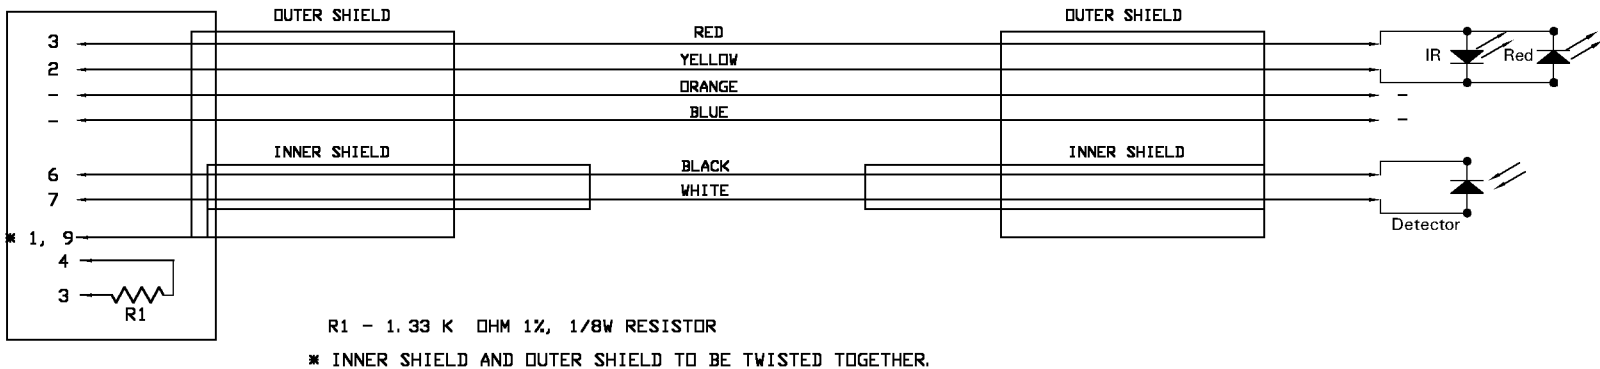

Title P860RA
Simed Baxter



Dim in mm

Tol ± 0.2

Scale Not To Scale

Drawn J.Nirwan

Date 17/02/03




Dwg No. SPF-860.1

Material :
Part No. 0018600

VIAMED Ltd.
15 Station Rd
Cross Hills, Keighley
West Yorkshire
BD20 7DT

Hypertronics Male 9 Pin

Finger Probe

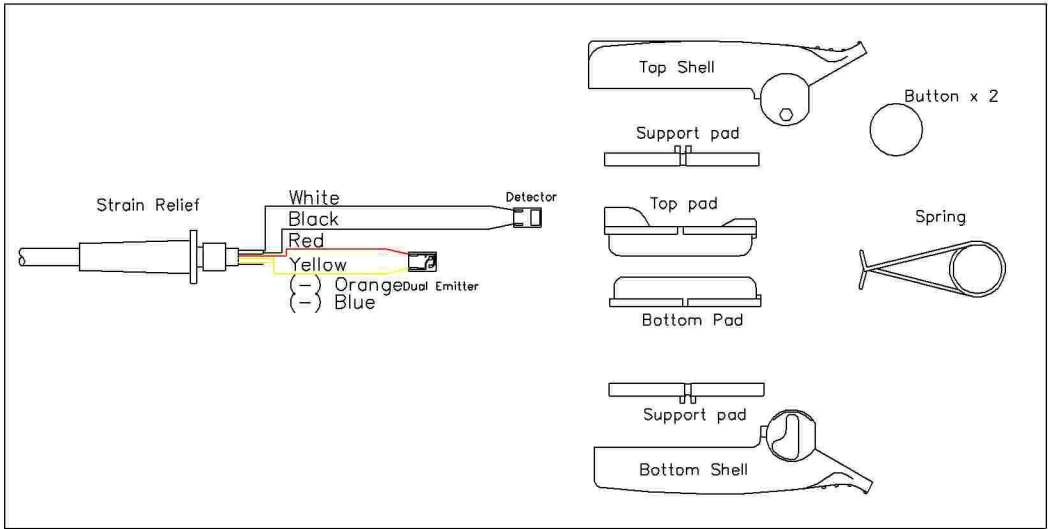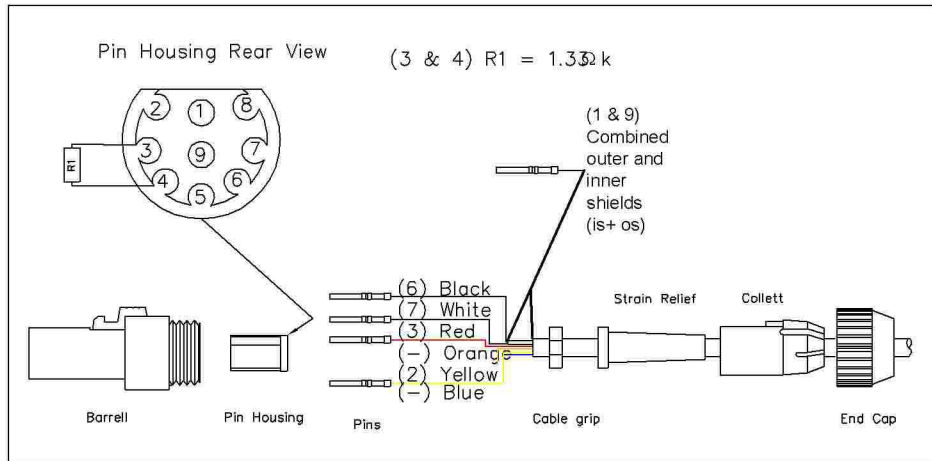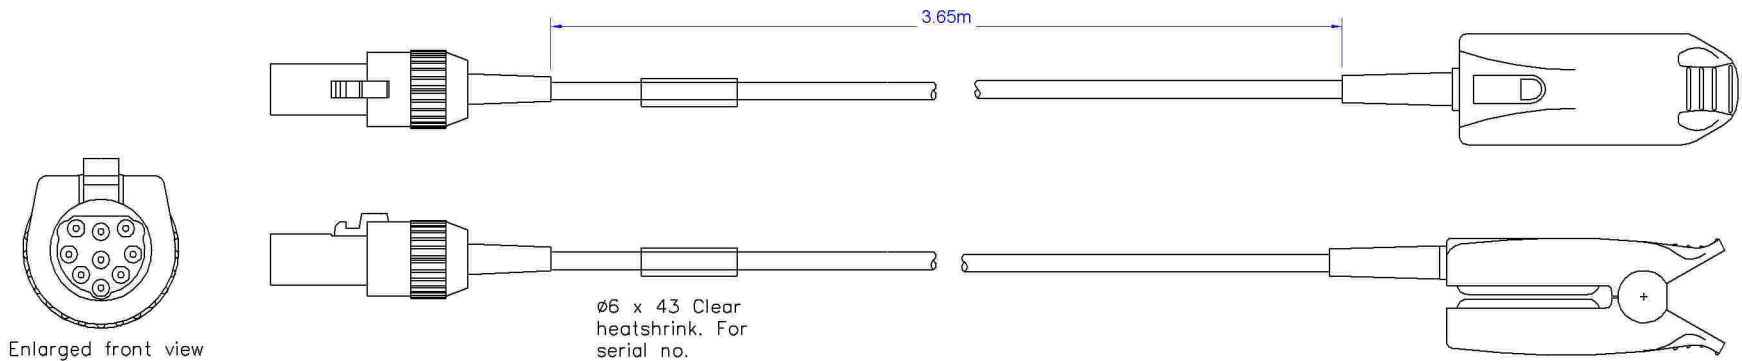

REV	Date	N*	Drawn	Approv	Material :
					Part No. 0018600

Title P860RA Simed Baxter			
Scale Not To Scale		Dim in	mm
Date 30/01/02		Tol	± 0.2
Dwg No. SPF-860		Drawn	J.Nirwan



VIAMED

Ltd.

15 Station Rd
Cross Hills, Keighley
West Yorkshire
BD20 7DT