



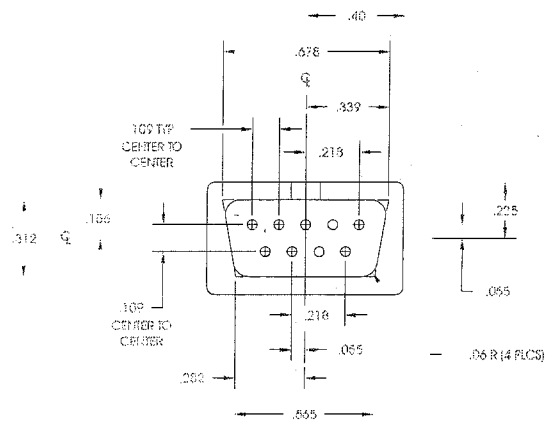



DETAIL A

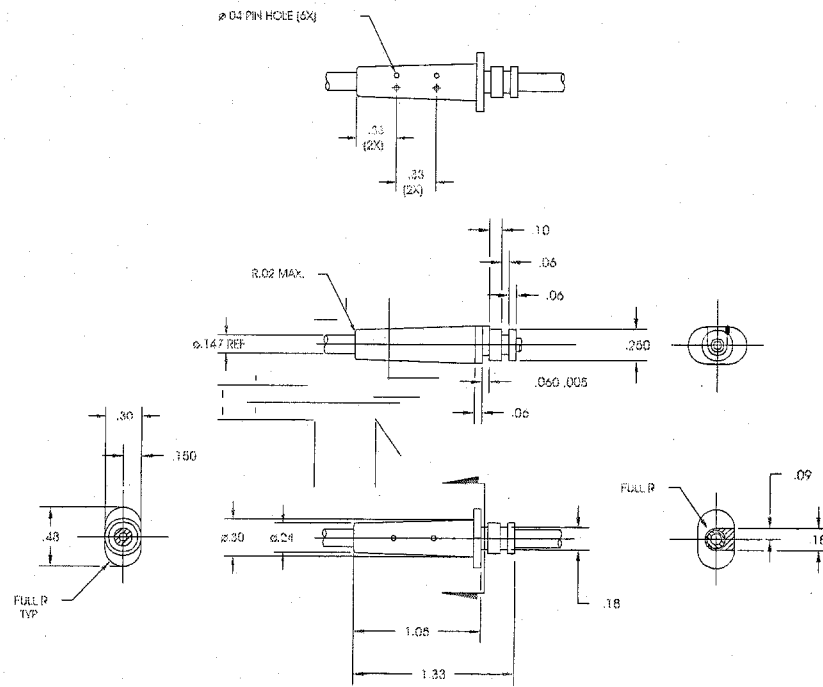


DETAIL B

REVISION LETTER


Finger Probe

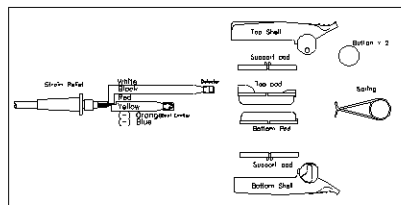


Finger Probe



Pre-Manufactured cable and

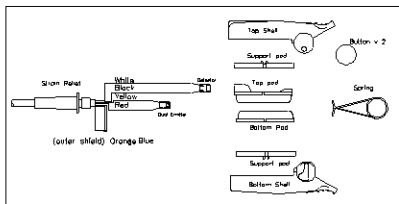

Finger Probe

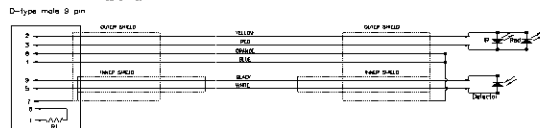


84 - 7.5 W OHM 1% 1/4W RESISTOR


* INNER SHIELD AND OUTER SHIELD TO BE TWISTED TOGETHER.

D-Type Male 9 Pin

Finger Probe

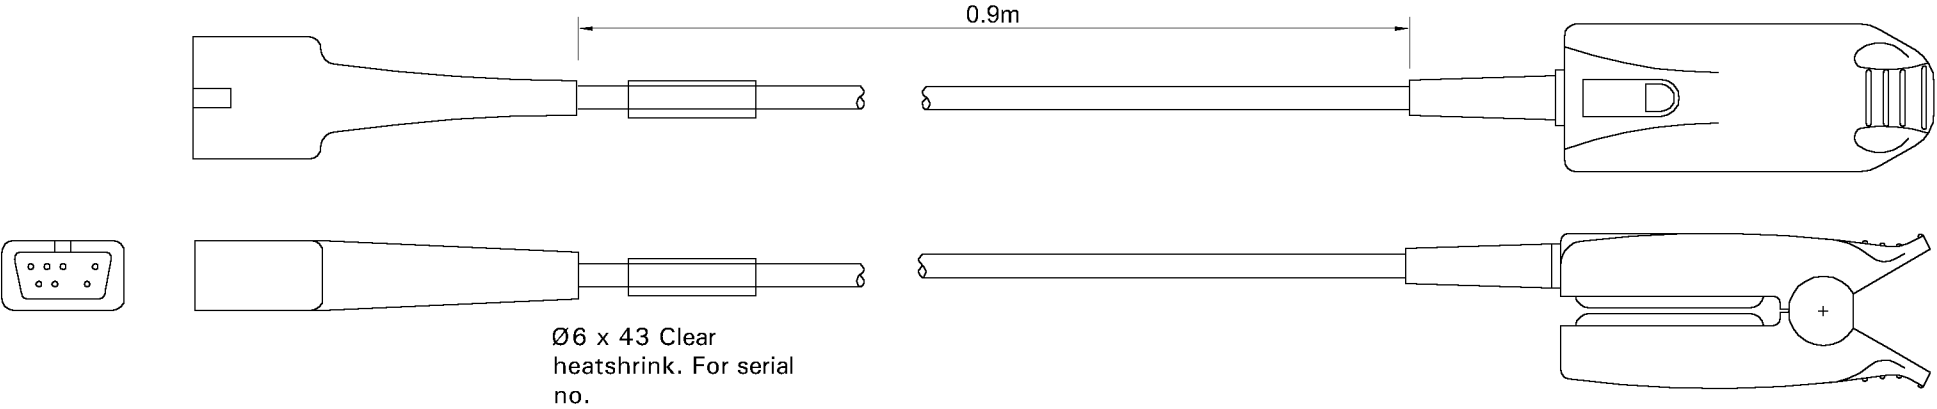

D-type male 9 pin

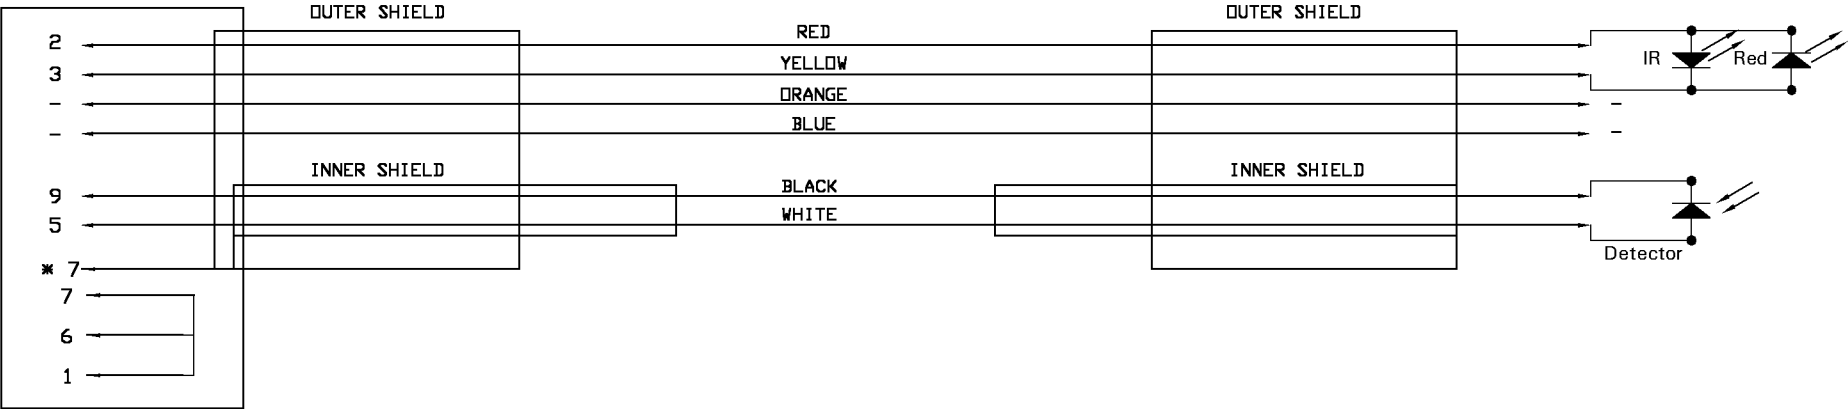


* INNER SHIELD AND OUTER SHIELD TO BE TWISTED TOGETHER.

Title		P861RA	
		BCI (Viamed)	
		Dim in	mm
		Tol	± 0.2
Scale		Not To Scale	Drawn
			J.Nirwan
Date		19/02/03	Dwg No.
			SPF-861.1


VIAMED Ltd.
15 Station Rd
Cross Hills, Keighley
West Yorkshire
BD20 7DT

REV	Date	Nº	Drawn	Approv	Material :
Part No.					0018610


D-Type Male 9 Pin

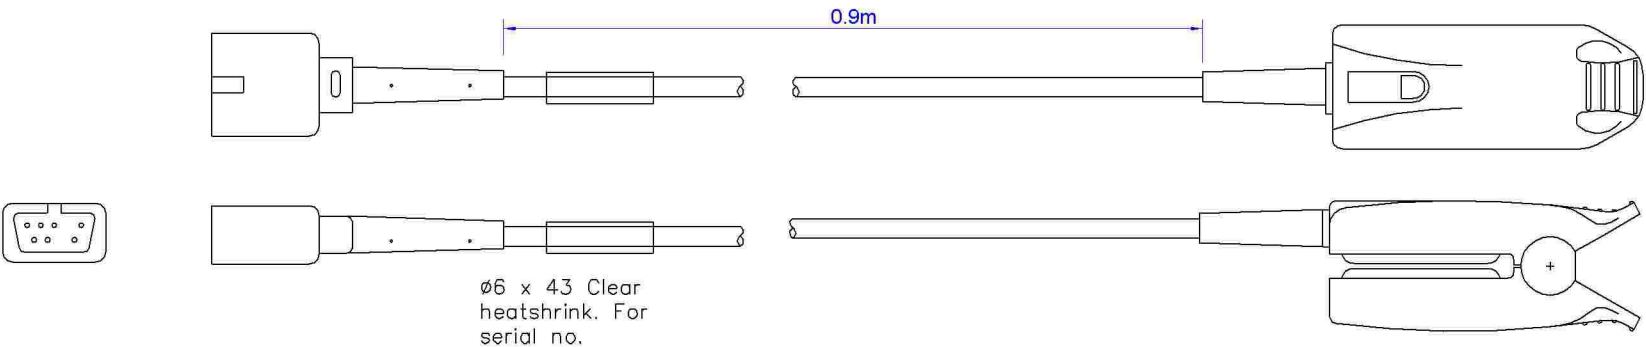


Finger Probe

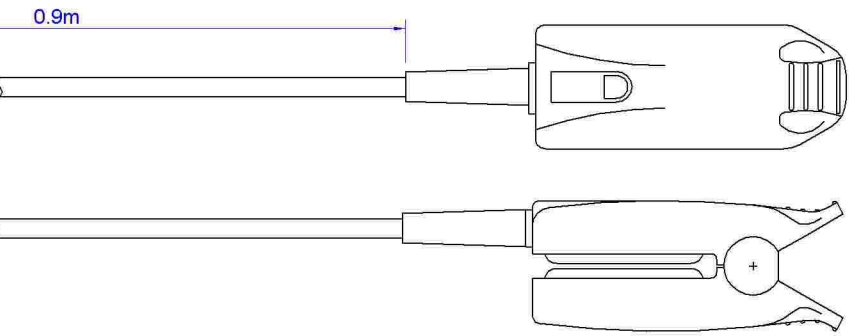

Connector Rear View

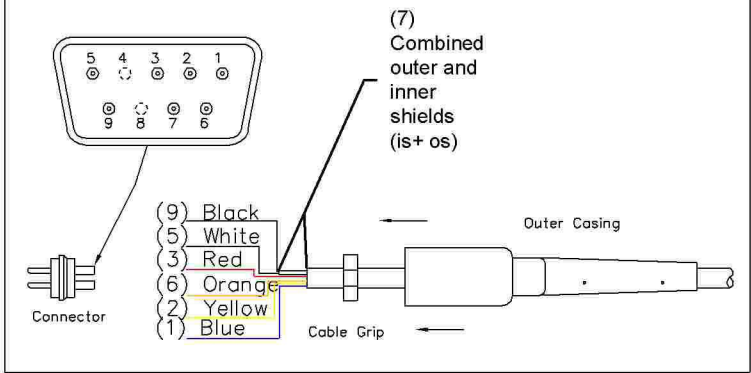


Pre-Manufactured cable end

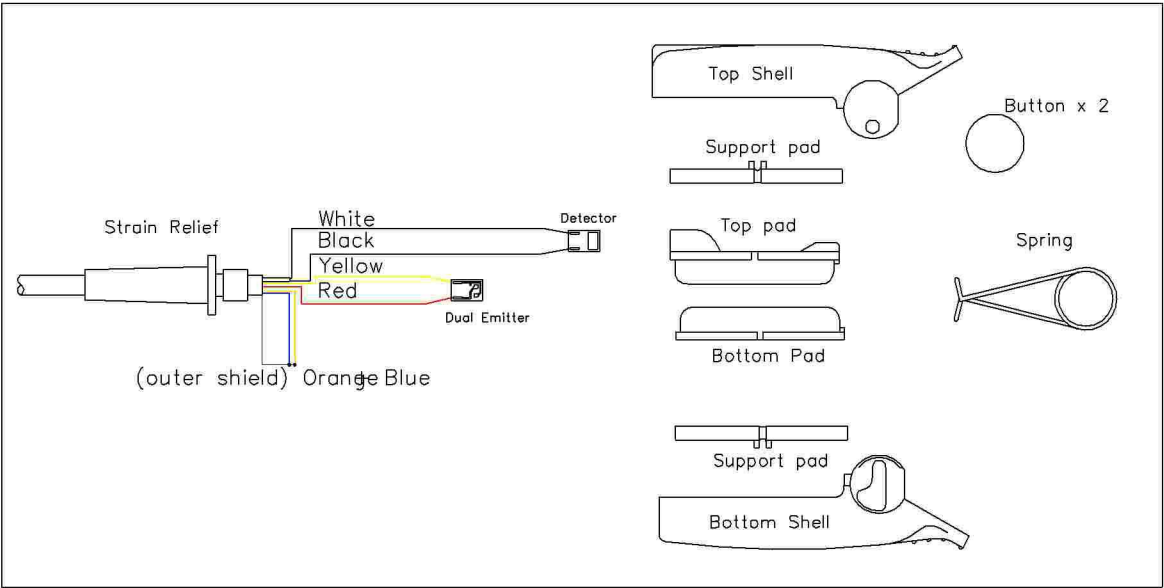


REV	Date	N*	Drawn	Approv	Material :
					Part No. 0018610

Title P861RA BCI (UDT)			
		Dim in	mm
Scale Not To Scale		Tol	± 0.2
Date 16/10/03		Drawn	K.J. Rush
Dwg No. SPF-861			
		15 Station Rd Cross Hills, Keighley West Yorkshire BD20 7DT	


D-Type Male 9 Pin

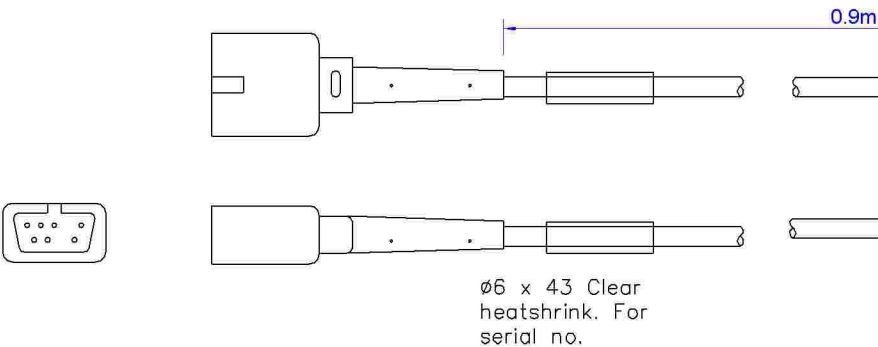


Finger Probe

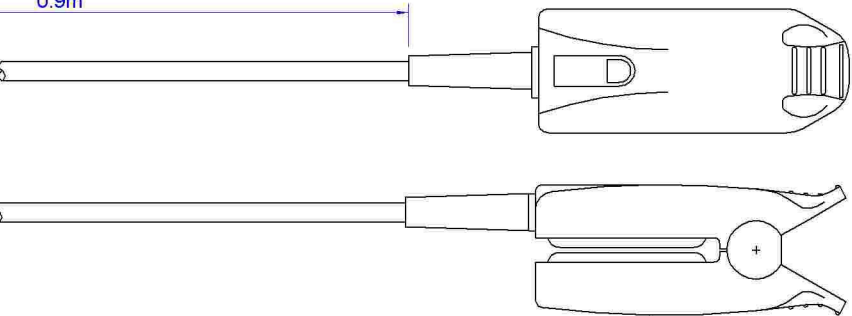


Connector Rear View

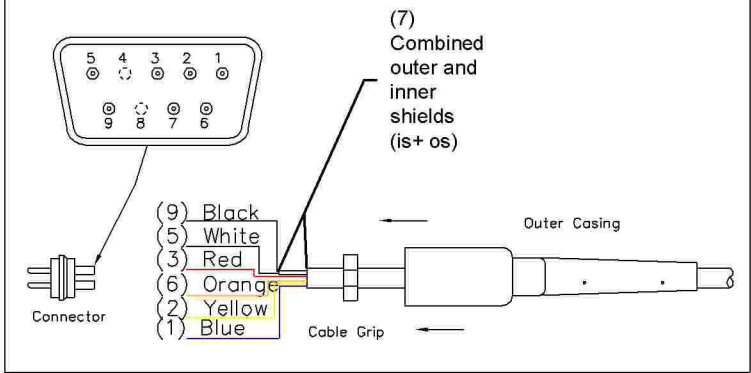

Pre-Manufactured cable end

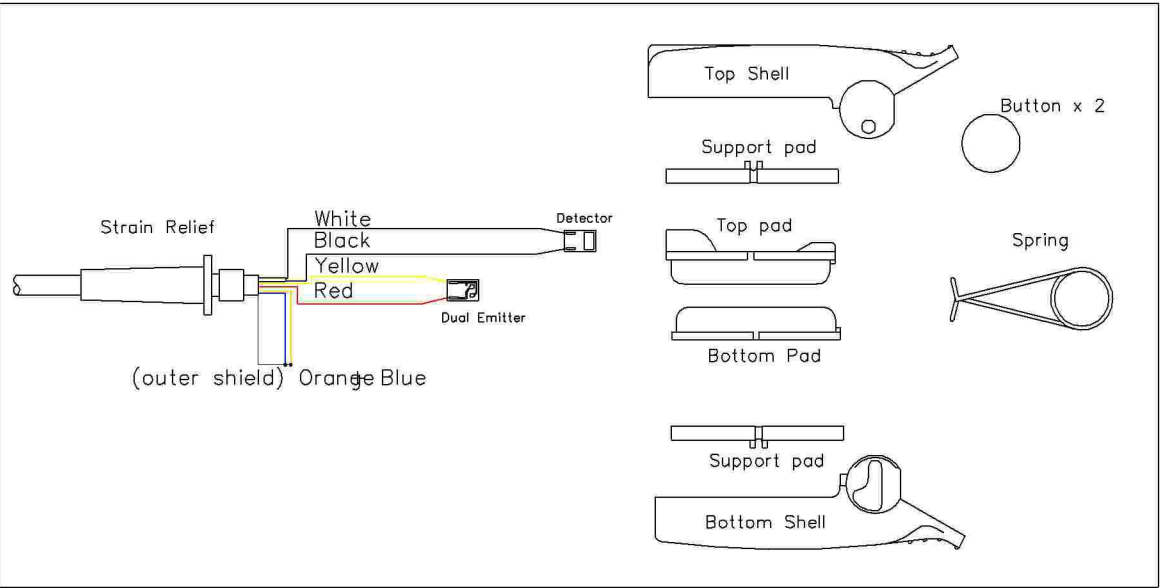

REV	Date	N*	Drawn	Approv	Material :
					Part No. 0018610

Title P861RA BCI (UDT)					VIAMED 15 Station Rd Cross Hills, Keighley West Yorkshire BD20 7DT	Ltd.	
Dim in		mm					
Tol		± 0.2					
Scale		Not To Scale					Drawn
Date		16/10/03		Dwg No.		SPF-861	