

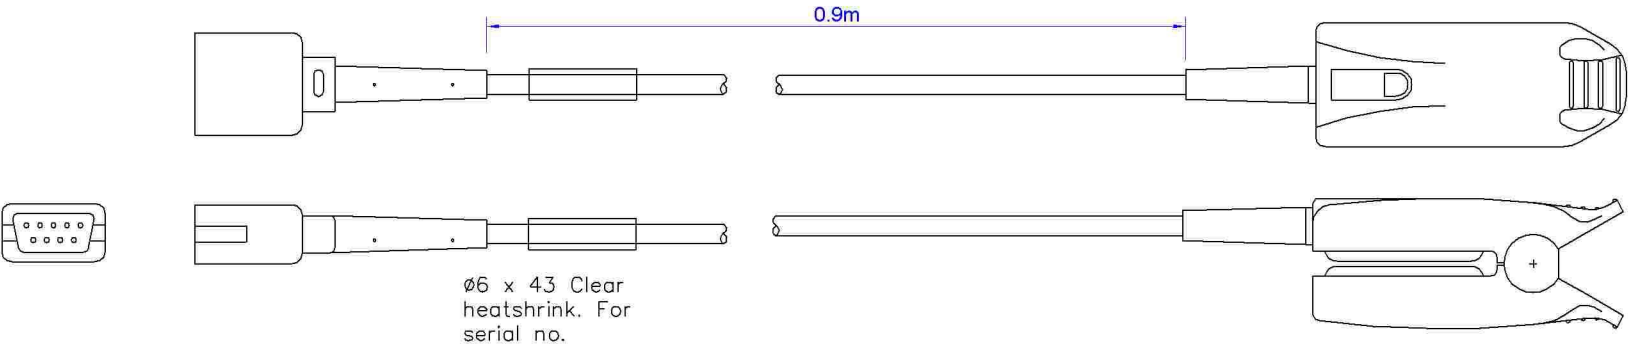
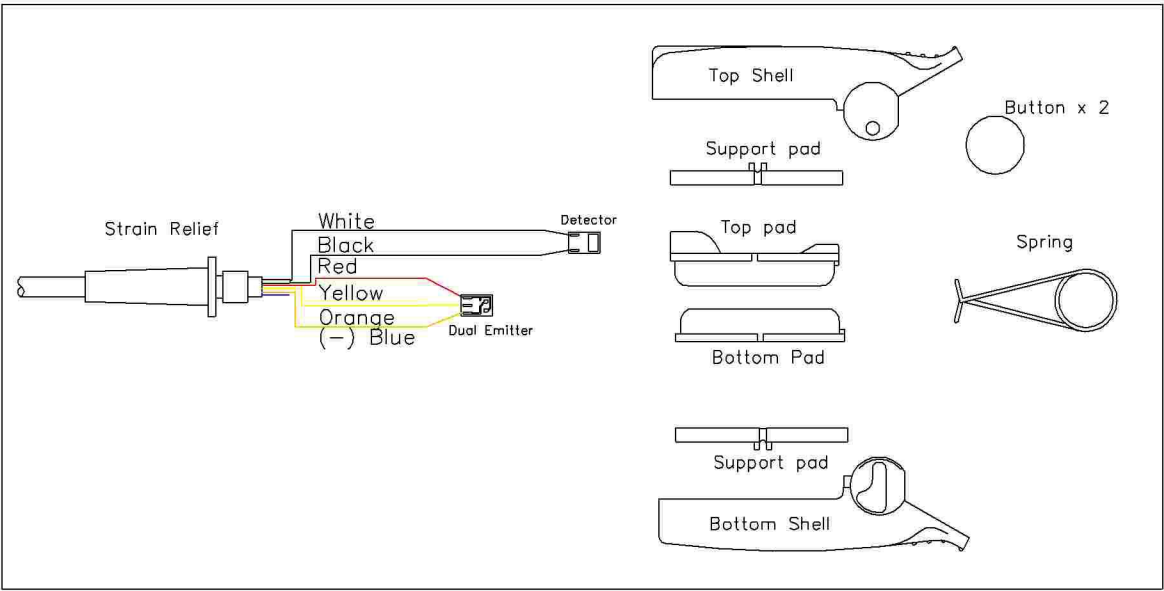


D-Type Male 9 Pin

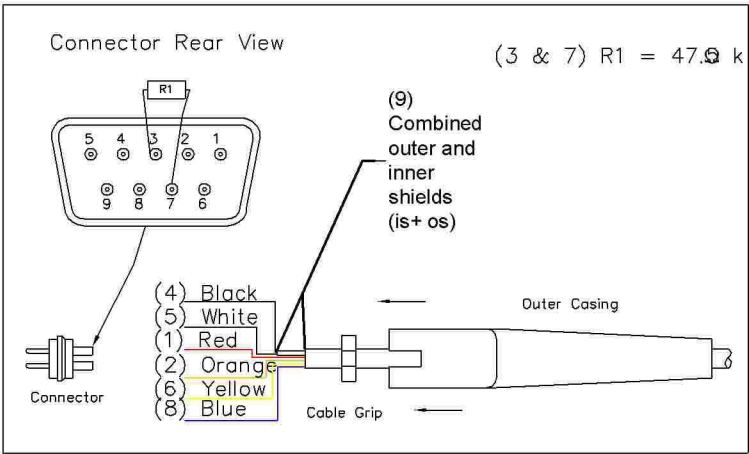

Finger Probe

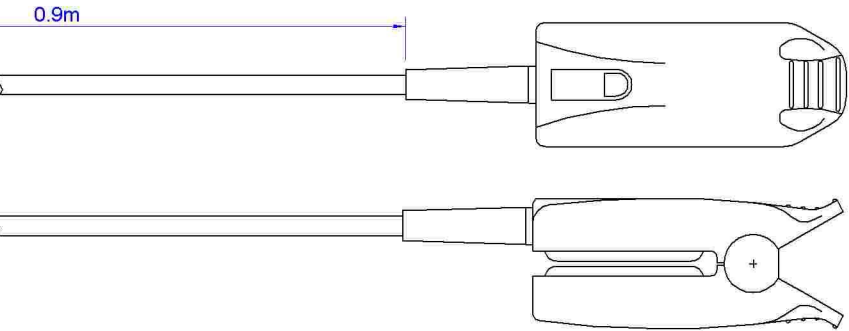

					Material :
REV	Date	N*	Drawn	Approv	Part No. 0018630

Title P863RA Datascope			
Dim in		mm	
Tol		± 0.2	
Scale	Not To Scale	Drawn	K.J. Rush
Date	16/10/03	Dwg No.	SPF-863




VIAMED

Ltd.


15 Station Rd
Cross Hills, Keighley
West Yorkshire
BD20 7DT

D-Type Male 9 Pin

Finger Probe

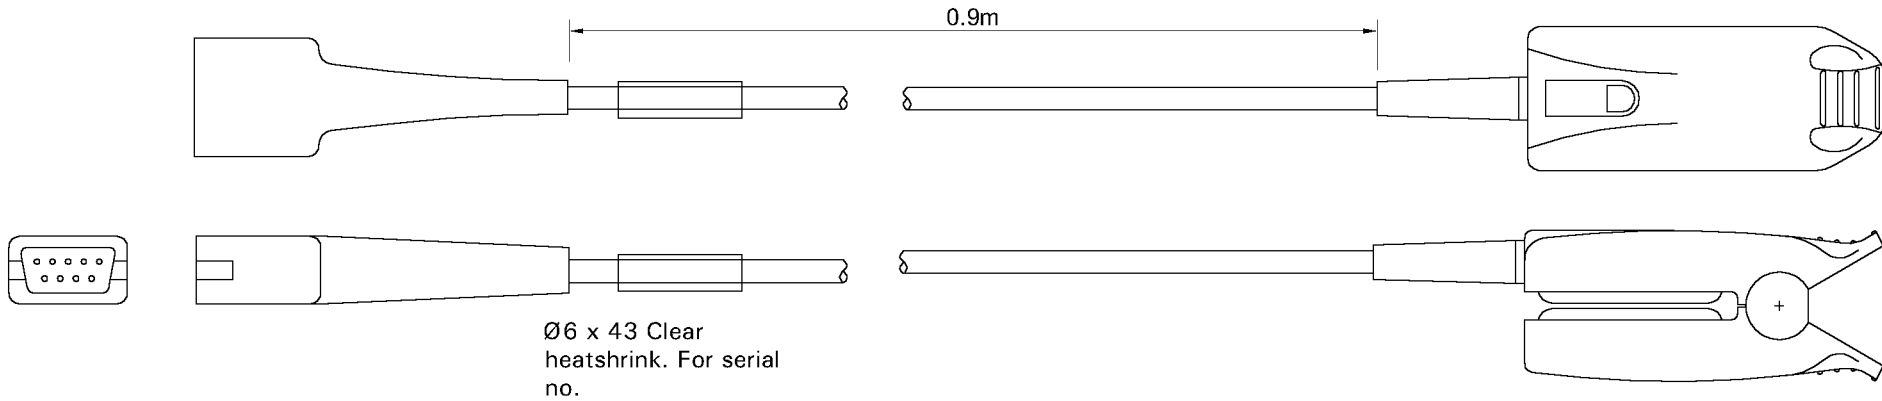

D-type male 9-pin

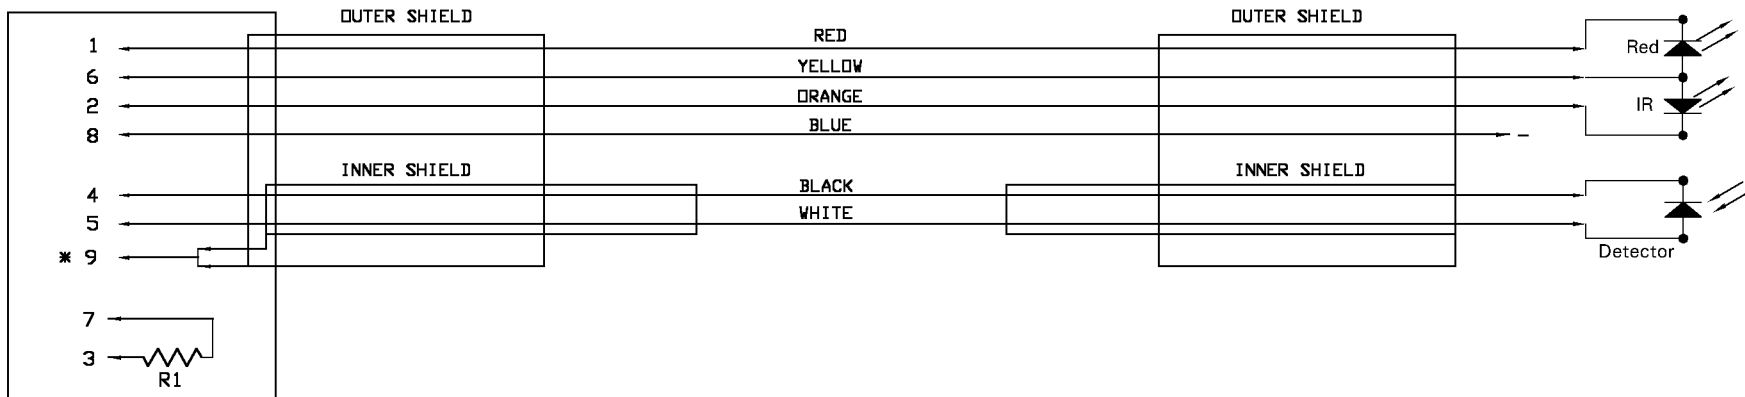

R1 - 47.5 K OHM 1%, 1/8W RESISTOR

* INNER SHIELD AND OUTER SHIELD TO BE TWISTED TOGETHER.

Title **P863RA**
Datascope



Dim in mm

Tol ± 0.2

Drawn J.Nirwan

Scale Not To Scale

Date 17/02/03

Dwg No. **SPF-863.1**


Material :


Part No. **0018630**

VIAMED Ltd.


15 Station Rd
Cross Hills, Keighley
West Yorkshire
BD20 7DT

REV Date N° Drawn Approv

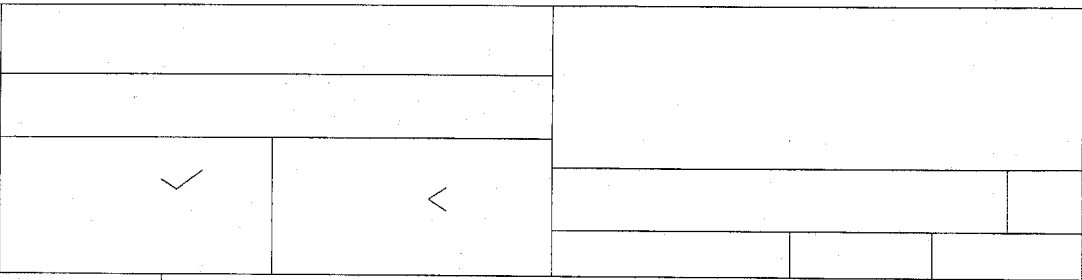

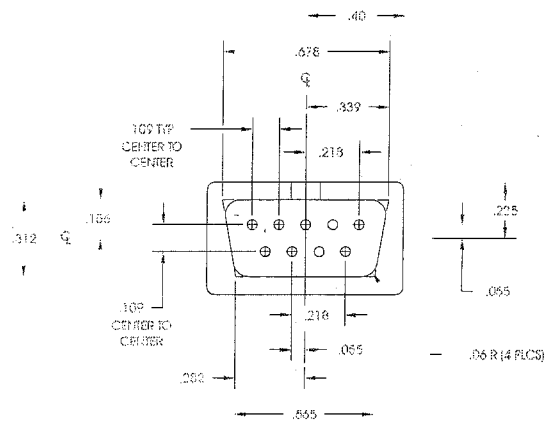

DETAIL A

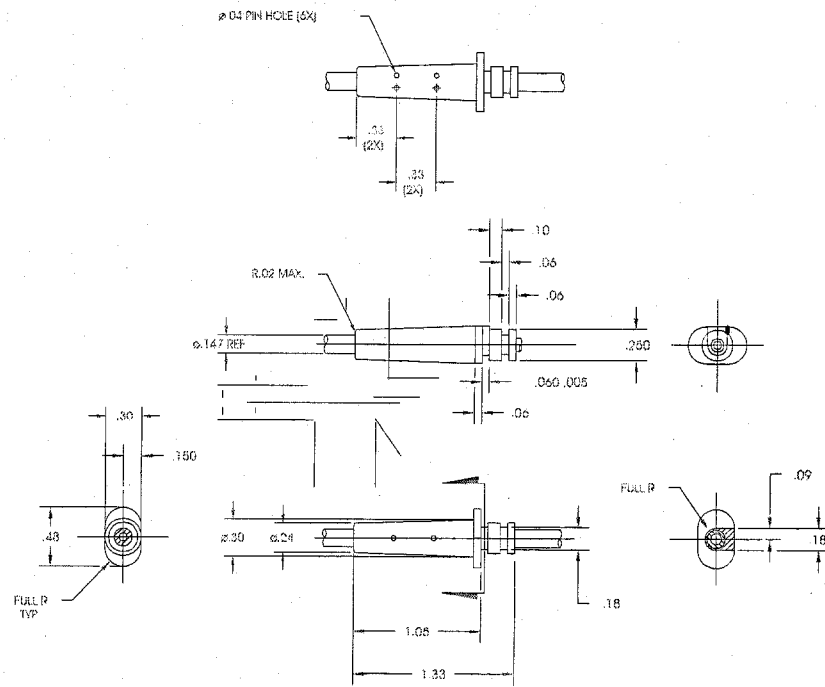

DETAIL B

REVISION LETTER