

Samples of SpO₂ Emitters and Detector configurations and types

'OEM' (Lead Frame)



'Viamed' (Lead Frame)



'Generic' manufacturer 'A' (Ceramic)

Old Version




'Generic' manufacturer 'B' (Ceramic)




'Generic' manufacturer 'A' (Ceramic)

New Version

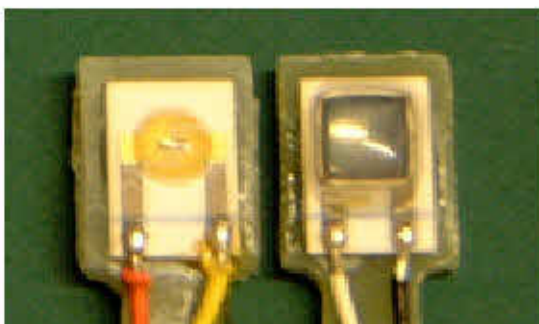


Spectrometry results of SpO₂ Emitters (Red and Infra Red)


'OEM' (Lead Frame)

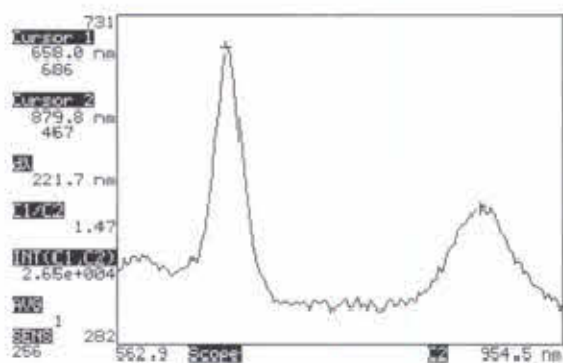

'Viamed' (Lead Frame)

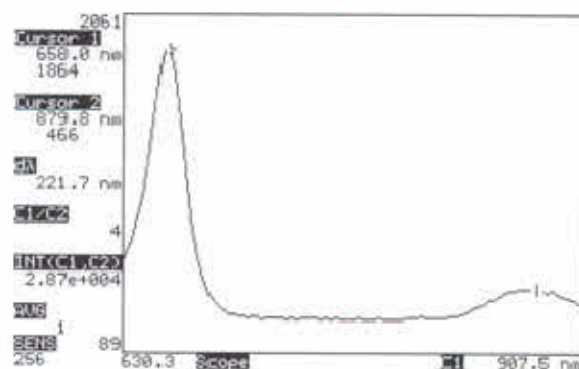

'Generic' manufacturer 'A' (Ceramic)

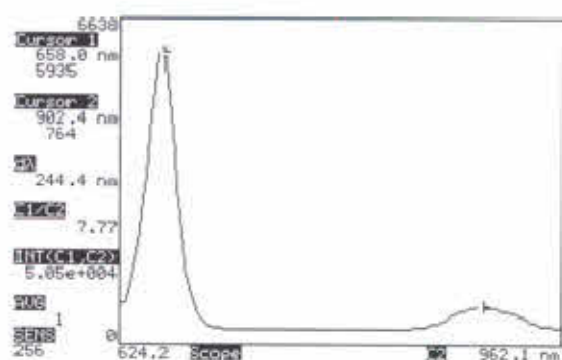

'Generic' manufacturer 'B' (Ceramic)

