



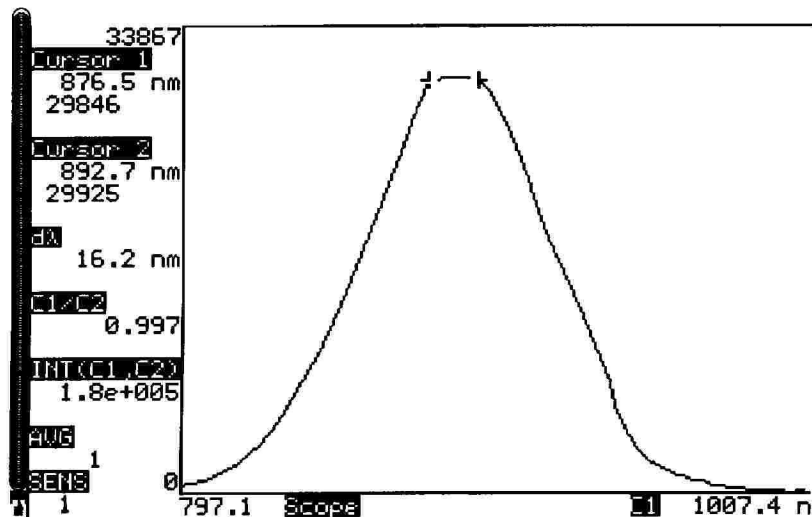

Spectrometer.	SPM 9001.
Manufacturer of Probe.	BCI.
Type.	Finger.
Part no.	Model 3044.
Serial no.	170271350
Connector.	9 pin male, D connector.
Connect to.	Oximeter or extension.
For use on.	
Tested on.	Nellcor N-200
Red peak wavelength (nm).	661.3.
Infrared peak wavelength (nm).	892.7 876.5 - 892.7.
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	05-01-00.

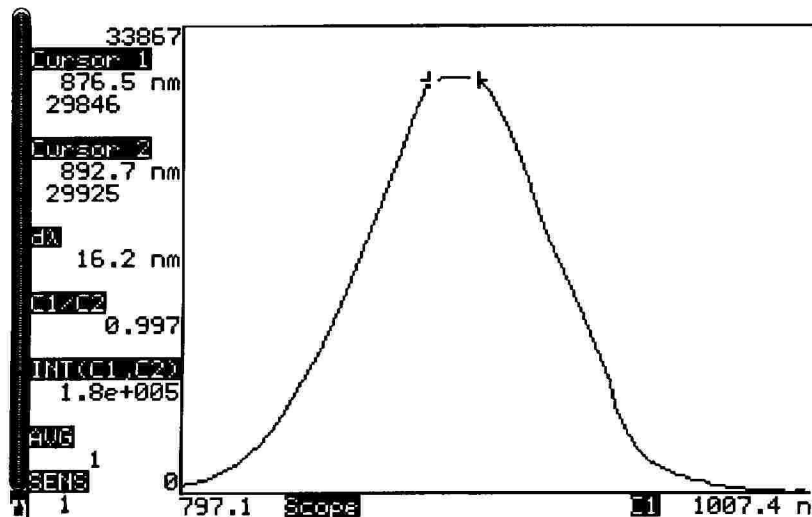

Spectrometer.	SPM 9001.
Manufacturer of Probe.	BCI.
Type.	Finger.
Part no.	Model 3044.
Serial no.	170271350
Connector.	9 pin male, D connector.
Connect to.	Oximeter or extension.
For use on.	
Tested on.	Nellcor N-200
Red peak wavelength (nm).	661.3.
Infrared peak wavelength (nm).	892.7 876.5 - 892.7.
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	05-01-00.