



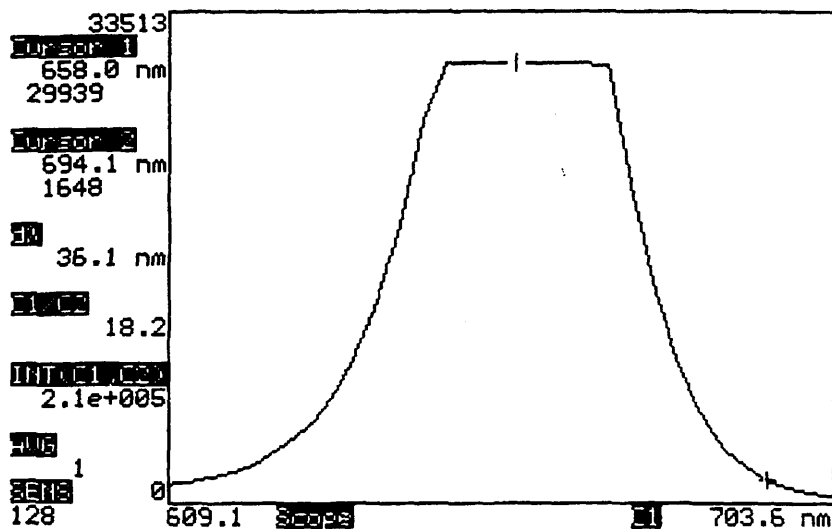

Spectrometer.	SPM 9001.
Manufacturer of Probe.	MSA Medical Products.
Type.	Finger.
Part no.	WS40349.
Serial no.	001960.
Connector.	5 pin male connector.
Connect to.	Oximeter or extension cable.
For use on.	MiniOX V oximeter.
Tested on.	MiniOX V oximeter.
Red peak wavelength (nm).	658.0.
Infrared peak wavelength (nm).	892.7..
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	14-12-99.

Notes.

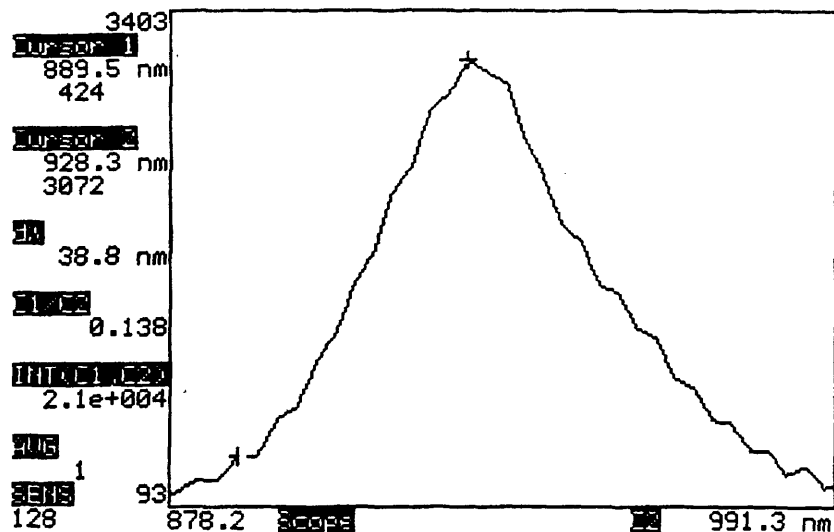

Spectrometer.	SPM 9001.
Manufacturer of Probe.	MSA Medical Products.
Type.	Finger.
Part no.	WS40349.
Serial no.	001960.
Connector.	5 pin male connector.
Connect to.	Oximeter or extension cable.
For use on.	MiniOX V oximeter.
Tested on.	MiniOX V oximeter.
Red peak wavelength (nm).	658.0.
Infrared peak wavelength (nm).	892.7..
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	14-12-99.

Notes.