



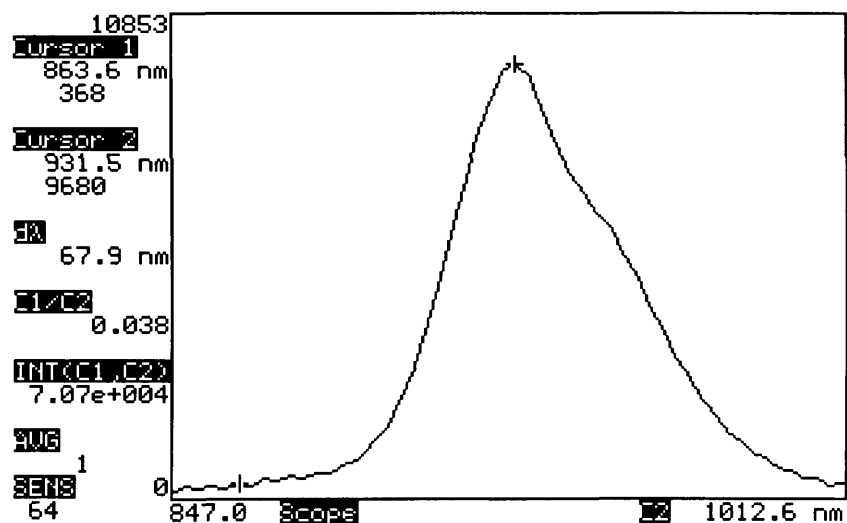

Spectrometer.	SPM 9001.
Manufacturer of Probe.	Novamatrix.
Type.	Finger.
Part no.	8660
Serial no.	33665.
Connector.	9 pin male.
Connect to.	Oximeter or extension.
For use on.	Novamatrix or compatible oximeters.
Tested on.	Novamatrix 515.
Red peak wavelength (nm).	661.3.
Infrared peak wavelength (nm).	931.5.
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	05-01-00.

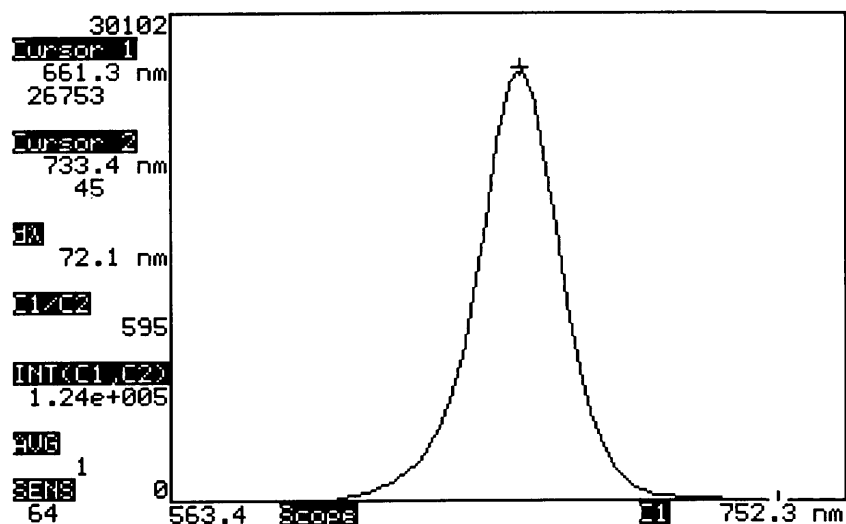

Spectrometer.	SPM 9001.
Manufacturer of Probe.	Novametrix.
Type.	Finger.
Part no.	8660
Serial no.	33665.
Connector.	9 pin male.
Connect to.	Oximeter or extension.
For use on.	Novametrix or compatible oximeters.
Tested on.	Novametrix 515.
Red peak wavelength (nm).	661.3.
Infrared peak wavelength (nm).	931.5.
Internal resistance value.	Unknown.
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	05-01-00.