



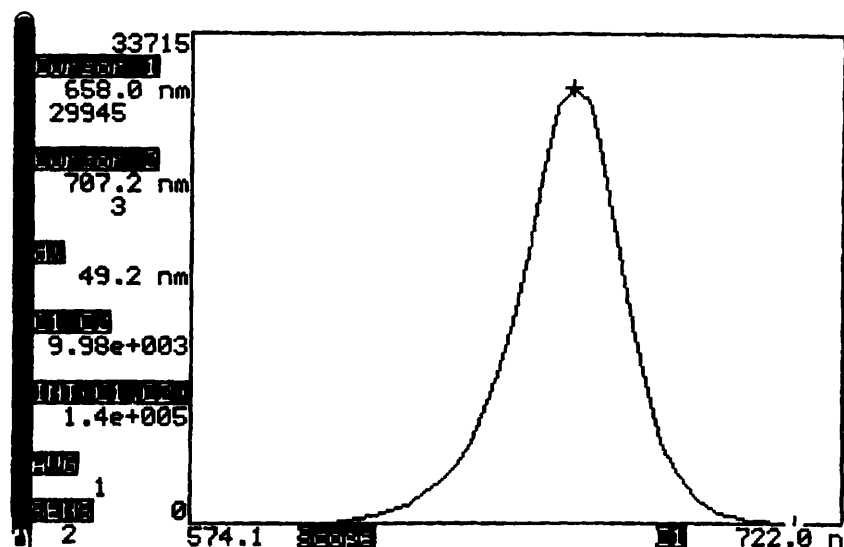

Spectrometer.	SPM 9001.
Manufacturer of Probe.	Datascope.
Type.	Finger.
Part no.	0600-00-0026-01
Serial no.	Da11515-F9.
Connector.	9 pin D type.
Connect to.	Oximeter or extension.
For use on.	Datascope oximeter or equivalent.
Tested on.	Datascope Accusat.
Red peak wavelength (nm).	658.0.
Infrared peak wavelength (nm).	928.3.
Internal resistance value.	Unknown
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	22-12-99.

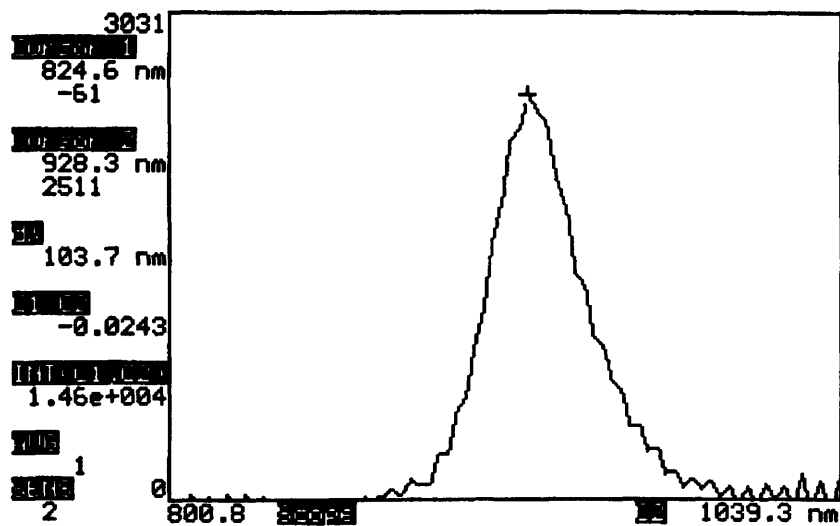

Spectrometer.	SPM 9001.
Manufacturer of Probe.	Datascope.
Type.	Finger.
Part no.	0600-00-0026-01
Serial no.	Da11515-F9.

For use on.	Datascope oximeter or equivalent.
Tested on.	Datascope Accusat.
Red peak wavelength (nm).	658.0.
Infrared peak wavelength (nm).	928.3.
Internal resistance value.	Unknown
Emitter configuration.	Unknown.
Carried out by.	S Watmough. I Eng., B Eng.
Date.	22-12-99.

