

Service Repair Sheet SRS68644

Contact Name

Company/ Hospital Name

Department

Position

Direct Phone

General Phone

Opera Account

Email

Order Number

Date Received

Booked in By

Main Company

Type Return

Samuel Strange

Nottingham University Hospital (C

Medical Equipment Service Unit (M

Assistant Technologist (Pneumatic

01159691169 Ext 59902

01159249924

00003930

samuel.strange@nuh.nhs.uk

12/Dec/2023

Robert Connor

Viamed

Quote

VIAMEDclean

Goods In Only

Decontamination
certificate provided
by customer ☐

Cleaned by Viamed,
if no declaration certificate
from customer ☒

Signed: RC
Date: 12/12/23

Goods Out Only

Cleaned by Viamed before
returning to customer

Signed: _____
Date: _____

Notes 04/Dec/2023 Kate Griffiths

04/Dec/2023 Kate Griffiths

Faulty display on MaxO2+A, s/n DD47799014. Unable to find s/n in i/stats

12/Dec/2023 Robert Connor

Received 1 x MAX-O2+A s/n DD47799014 with flow diverter.

Ready For quote

CANON 19.12.23

Repair Complete Signed

SRN	Equipment	Stock Ref	Serial Number	Warranty
SRN36159	Oxygen Analyser		DD47799014	N

0140050 x 1

S/N, SRS, SRN

unable to repair

0111260 x 1 @ £372

New unit

UPS x 1 @ £12

SS/MC/1289500
Returns Ref: SRS68644

City Campus
Clinical Engineering
Hucknall Road
Nottingham
NG5 1PB

Tel: 0115 969 1169 Ext: 82505
E-mail: mesusupport@nuh.nhs.uk

5th December 2023

Viamed Limited
15 Station Road
Cross Hills
Keighley
BD20 7DT
F.A.O. Kate Griffiths

Dear Kate

Non-Warranty Repair

Asset No	151069
Manufacturer	Maxtec
Model	MaxO2+A
Serial Number	DD47799014
Perceived Fault	Faulty display

The above item has been returned to you under non-warranty repair.

Could you please contact our Chief Technician Mr Richard Tuckwood on extension number 82505 or email mesusupport@nuh.nhs.uk or Adam.Keeton@nuh.nhs.uk with the cost of repair and confirmation for the work to go ahead. A purchase order number will then be issued to cover the cost of the repair.


Yours sincerely,

P. P. M. E. Chesters

Mr Richard Tuckwood
MESU Team Leader
MESU City Campus

Catherine Spence Required Reading **1 Calls** 35 Issues **23 Unread**
 21 ISO Tasks | **My Requests** 20.00 °C

RS Full, ZT Full, CS Half , CH 03:30:00 PM For 2 Hours, AM Full

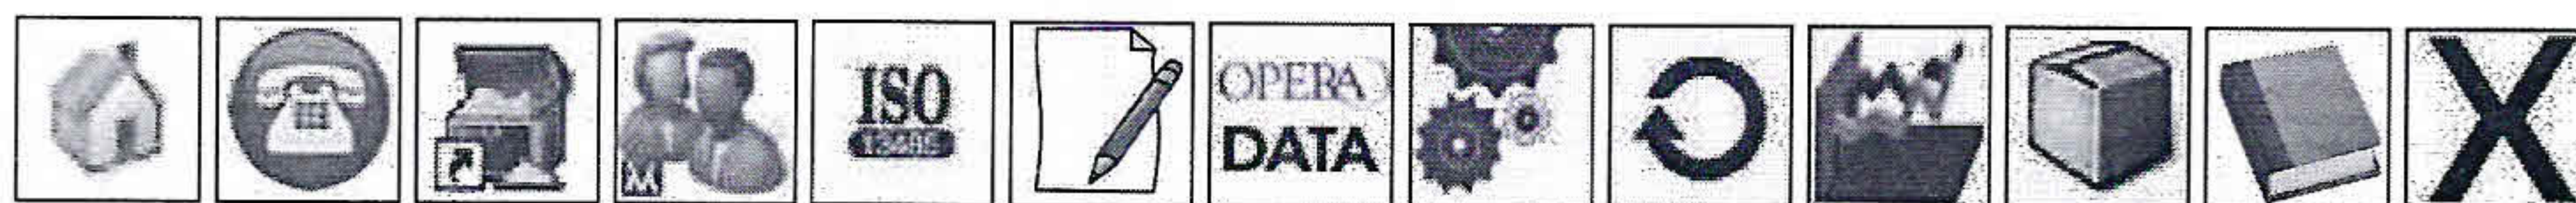

Nottingham University Hospital (Queens Medical Centre Campus)

CID4013 Opera 00003930
 Type:NHS Hospital End User
 Nottingham University Hospital (Queens Medical Centre Campus) ,
 Derby Road, Nottingham, , NG7
 2UH, UK
 Tel 01159249924 GBP End User
 (0001) [Log Call](#) [Add Issue](#)
 Credit Credit Cr 30 Days after date
 of invoice Credit Limit 0.00GBP



Use :0001 GBP End User

Repair SRS68644 Values in Pounds @ £1: £1.00

SRN36159	Oxygen Analyser	0111260			
	Parts Required	Reference	Quantity	Unit Cost	Total Line
		0111260	1	£372.00	£372.00
				Parts Cost	£372.00

**Page updated, TRipple check prices to price
in intrastats main search**

CHECK PRICES BEFORE SENDING QUOTE

Quote Sent