





VIAMED



PHOTOTHERAPY LIGHT SHIELD TECHNICAL DATA SHEET.

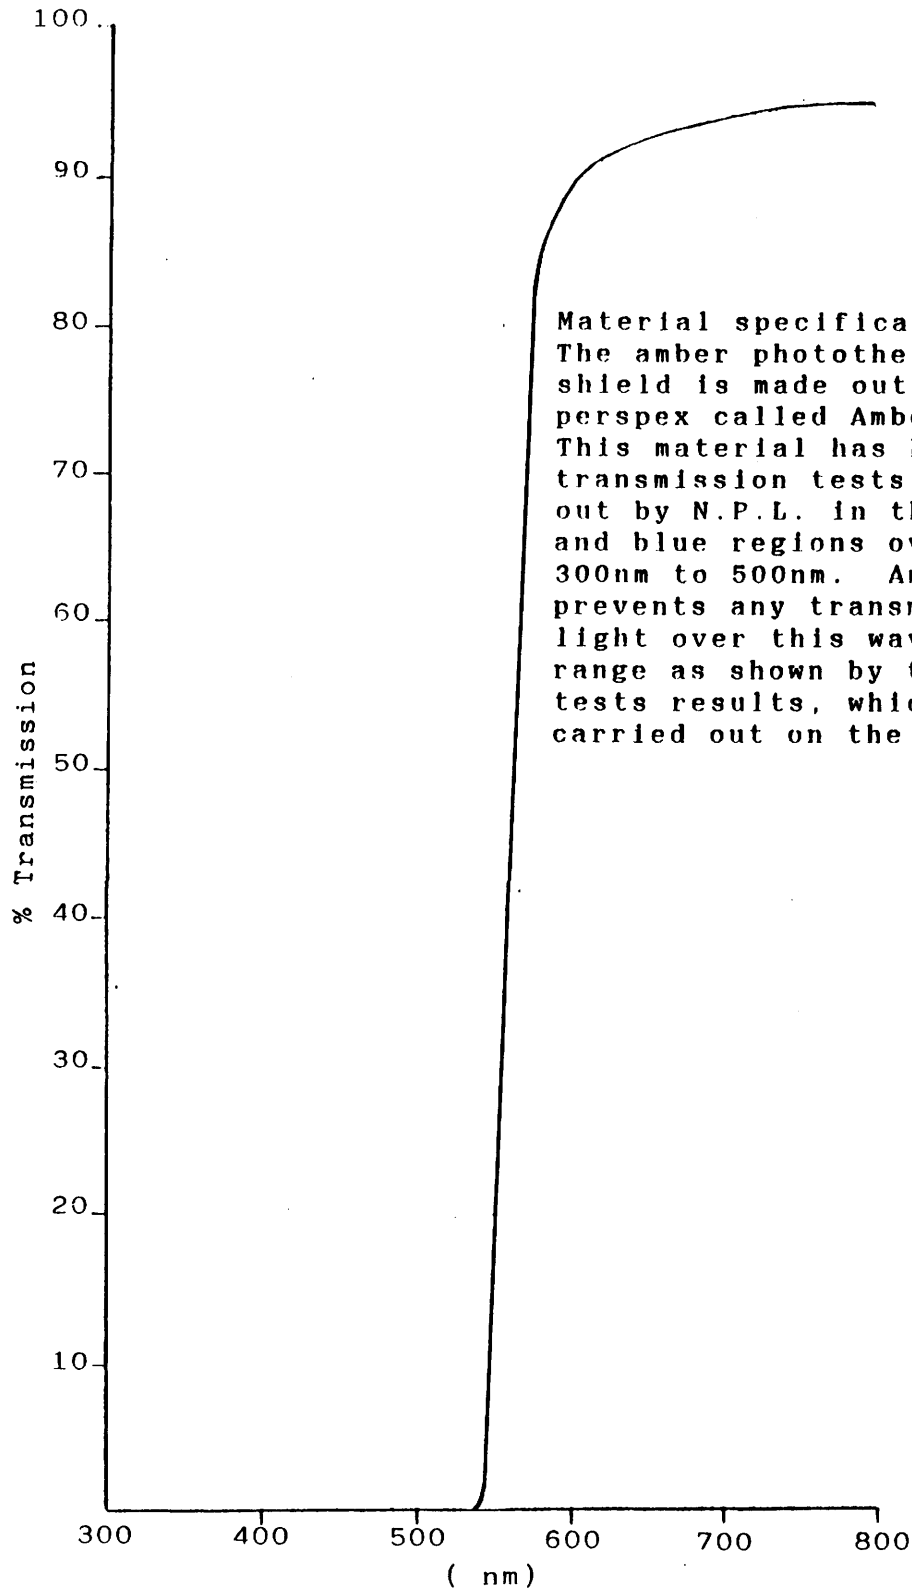

Material specification:
The amber phototherapy light shield is made out of I.C.I. perspex called Amber 300. This material has had light transmission tests carried out by N.P.L. in the U.V. and blue regions over the range 300nm to 500nm. Amber 300 prevents any transmission of light over this wavelength range as shown by the N.P.L. tests results, which were carried out on the 12.11.88.



**Viamed Limited, 15 Station Road, Cross Hills,
Keighley, West Yorkshire BD20 7DT**
Tel: 01535 634542 / 636757 Fax: 01535 635582
Registration No. 1291765 in England