



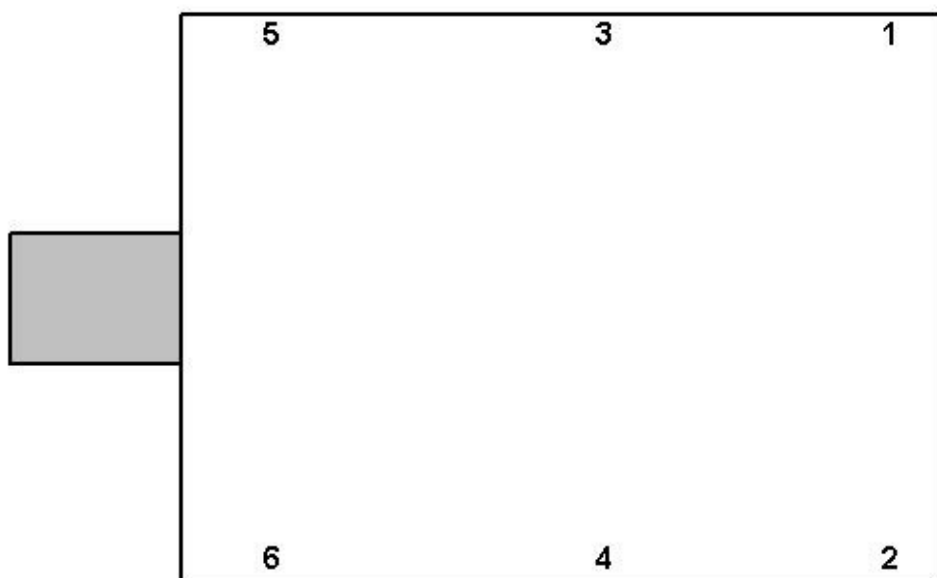

Libra			Results deg C				Avg
T1	35.6	34.8	36.4	36.5	36.8	37.1	36.2
T2	35.1	35.3	37	37.1	36.8	37.1	36.4
T3	33.3	35.1	37.2	36.4	35.3	38	35.9
T4	34.6	34.4	36.5	38	37.8	37.2	36.4
T5	35.5	36.4	37	38	36.5	37.1	36.8
T6	37.5	37.9	38	38.5	38	37.7	37.9

Fluke			Results deg C				Avg
T1	35.6	39.4					37.5
T2	37.6	38.9					38.25
T3	36	38.3					37.15
T4	35.8	39.5					37.65
T5	37.8	36.8					37.3
T6	39	38.9					38.95

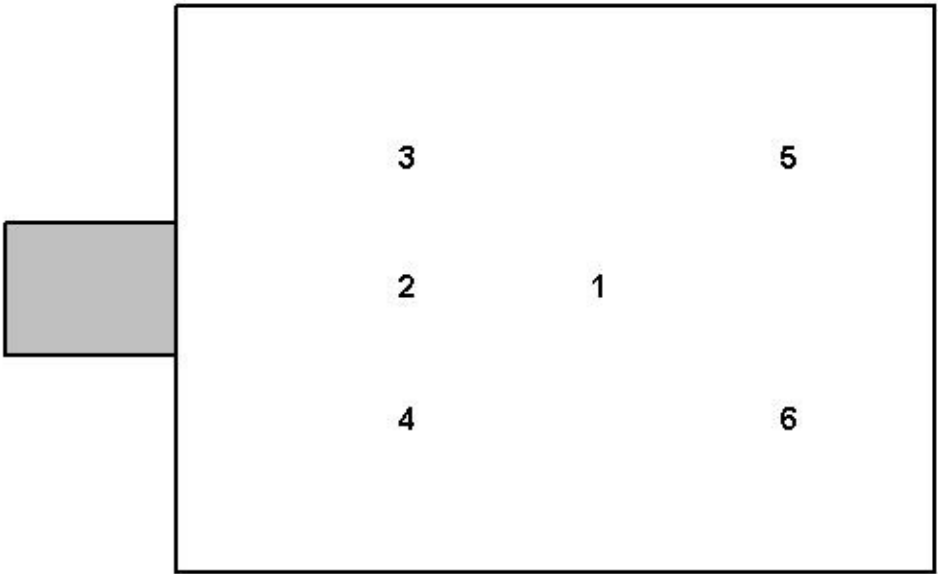

Fluke	Room temp		Results deg C				Avg
T1	24.5	36.6	36.6	37.9	38.7	38.7	37.7
T2	24.5	36.1	36.3	36.7	37.3	37.5	36.78
T3	24.5	37.4	37.5	37.6	38.5	38.5	37.9
T4	24.5	37.2	36.4	36.3	36.7	36.9	36.7
T5	24.5	36	36	37.2	37.4	37.1	36.74
T6	24.5	36.8	37.2	37.9	37.7	38.1	37.54