


Overview - device and packaging labels for CapnoTrue AMP / ASP / MG

All parts in the scope of supply are packed in a transportation carry case with label attached outside (see images below):

1) Universal Case back label (same for CapnoTrue AMP/ASP/MG)

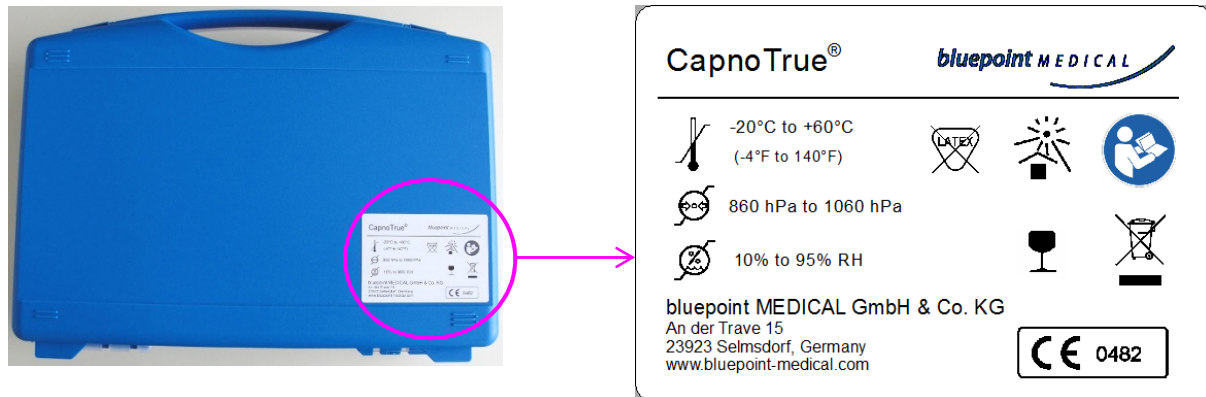

2) Serial number label (different for each device)



3) Case side label – REF, HIBC (different for each model, see table below)



Starter Kits can be ordered with selectable SpO₂ sensor. The REF and HIBC code depends on the sensor type ordered.

Find below a list of all available Starter Kit versions:

Device	+ Sensor	REF (Order number)	HICB Code
CapnoTrue AMP	SC 6500 (SoftCap)	3090112001-SC	+EBPM3090112001SC0+
	SCA 6500 (SoftCap autoclavable)	3090112001-SCA	+EBPM3090112001SCA08
	W 6500 (Wrap Sensor)	3090112001-W	+EBPM3090112001W0X
	SCP 6500 (SoftCap pediatric)	3090112001-SCP	+EBPM3090112001SCP0N
	SCPA 6500 (SoftCap autoclavable pediatric)	3090112001SCPA	+EBPM3090112001SCPA0X
	SF 6500 (SoftFlap)	3090112001-SF	+EBPM3090112001SF01
CapnoTrue ASP	SC 6500 (SoftCap)	3090112002-SC	+EBPM3090112002SC0%
	EP 6500 (Ohrsensor)	3090112002-EP	+EBPM3090112002EP0+
	SCA 6500 (SoftCap autoclavable)	3090112002-SCA	+EBPM3090112002SCA09
	W 6500 (Wrap Sensor)	3090112002-W	+EBPM3090112002W0Y
	SCP 6500 (SoftCap pediatric)	3090112002-SCP	+EBPM3090112002SCP0O
	SCPA 6500 (SoftCap autoclavable pediatric)	3090112002SCPA	+EBPM3090112002SCPA0Y
	SF 6500 (SoftFlap)	3090112002-SF	+EBPM3090112002SF02
CapnoTrue MG	SC 6500 (SoftCap)	3090112009-SC	+EBPM3090112009SC06
	SCA 6500 (SoftCap autoclavable)	3090112009-SCA	+EBPM3090112009SCA0G

4) Case Inlay Label - Model/Type label (different for each model, see table below)



5) Device Label (different for each model, see table below)

For position of back label see device below (front and back):



Device labels (CapnoTrue AMP, ASP, MG):



DOCUMENT HISTORY

Rev.	Date	Issued by	Description of changes
1	15.10.2009	H. Fröhlich	Initial version (started at rev.1)
2	14.03.2012	H. Fröhlich	- Update labels - Included HIBC code - reduce to label generated at bluepoint (remove IRMA, Airway adapter, Li-Ion battery etc. labels)
3	02.03.2015	H. Fröhlich	- update device label (60601-1 3rd Ed. req.)
4	07.04.2015	H. Fröhlich	- Adapt to new packaging in carry case - Change layout