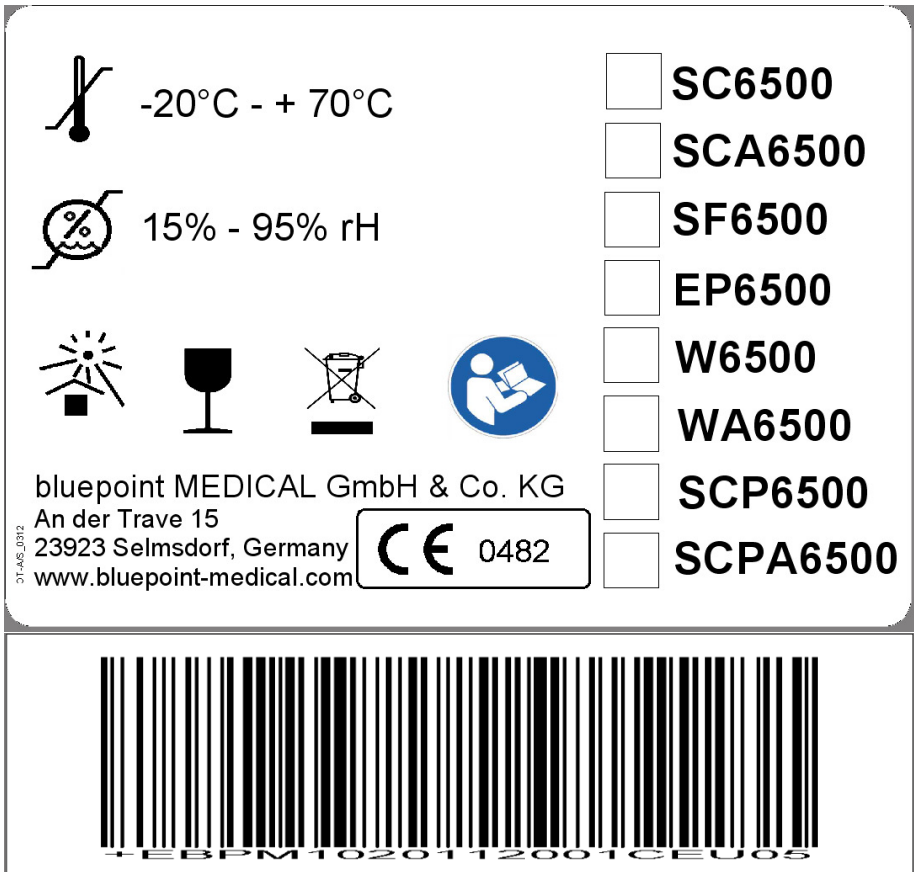



bluepoint MEDICAL	DMR	Rev.: 2
Internal Document	4.9_Labeling	Page 1 of 3

Overview about device and packaging labels for OxyTrue A and OxyTrue S:

OxyTrue A	
Device label	 The device label for OxyTrue A includes the following information: OxyTrue[®]A and IP32 REF 1020112001 SN T80600186 CE 0482 - bluepoint MEDICAL GmbH&Co.KG, Germany, www.bluepoint-medical.com 2014-08 - Icons: a person reading a document, a person walking, and a crossed-out trolley.
Box bottom label	 The box bottom label for OxyTrue A includes the following information: - Temperature range: -20°C - + 70°C (with thermometer icon) - Humidity range: 15% - 95% rH (with humidity icon) - Icons: a crossed-out light source, a glass, a crossed-out trolley, and a person reading a document. - bluepoint MEDICAL GmbH & Co. KG, An der Trave 15, 23923 Selmsdorf, Germany, www.bluepoint-medical.com CE 0482 - Selection of models (each with a checkbox): ☐ SC6500 ☐ SCA6500 ☐ SF6500 ☐ EP6500 ☐ W6500 ☐ WA6500 ☐ SCP6500 ☐ SCPA6500 - Barcode: +EBPM1020112001CEU05

bluepoint MEDICAL	DMR	Rev.: 2
Internal Document	4.9_Labeling	Page 2 of 3

Box side label (REF and serial number)	S/N  REF 
OxyTrue S	
Device label	OxyTrue® S IP32 REF 2020112011 SN T80600186 CE 0482 bluepoint MEDICAL GmbH & Co. KG Germany www.bluepoint-medical.com 2014-08
Box bottom label	 -20°C - + 70°C  15% - 95% rH     bluepoint MEDICAL GmbH & Co. KG An der Trave 15 23923 Selmsdorf, Germany www.bluepoint-medical.com CE 0482 ☐ SC6500 ☐ SCA6500 ☐ SF6500 ☐ EP6500 ☐ W6500 ☐ WA6500 ☐ SCP6500 ☐ SCPA6500

Created: H. Fröhlich	Date: 02.03.2015
4.9.0_overview_labeling_rev2.docx	

bluepoint MEDICAL	DMR	Rev.: 2
Internal Document	4.9_Labeling	Page 3 of 3

	
Box side label	S/N  REF 

Created: H. Fröhlich	Date: 02.03.2015
4.9.0_overview_labeling_rev2.docx	