

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 1 von 29

Issued	Signature	Date
Rayk Jürgensen		
Reviewed	Signature	Date
Approved	Signature	Date
Bernd Lindner		

Document History Log

Rev.	Date / By	Modifications
0	13.04.2015 / RJ	Initial version

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 2 von 29


1. Label Layout: VIA Connector Sampling Lines

Dimension Inlay: 105 mm x 100 mm


Dimension Box Label: 68 mm x 99 mm

Ref.: 4420800, Typ: P-S-VIA-200

Single Port Nasal Prong, Adult, Short Term

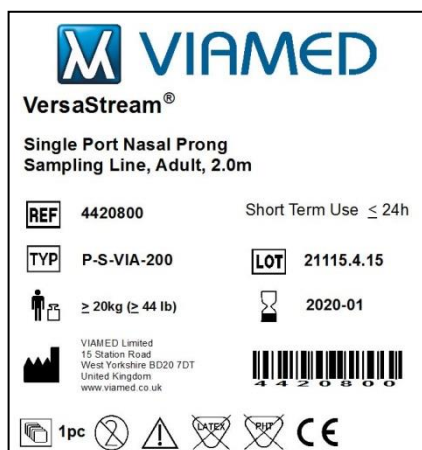


Front view

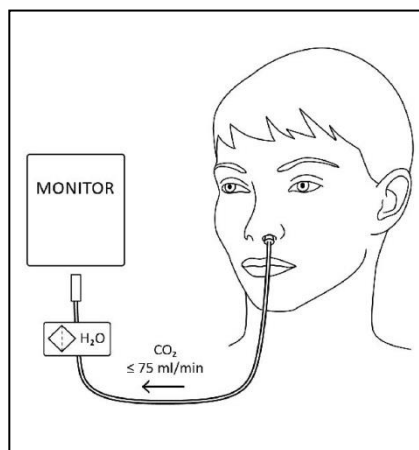

Rear view

Box Label

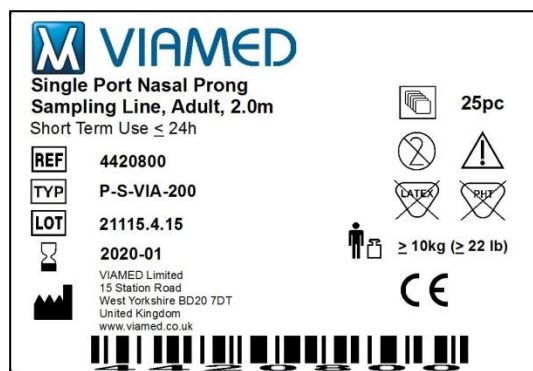


bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 3 von 29

Ref.: 4420801, Typ: NA-S-VIA-200
Nasal Sampling Line, Adult, Short Term




Front view

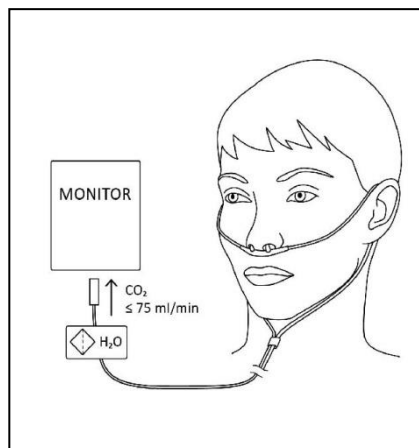

Rear view


Box Label

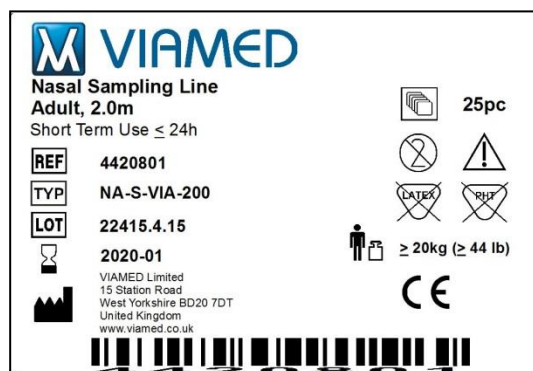


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 4 von 29

Ref.: 4420802, Typ: NP-S-VIA-200
Nasal Sampling Line, Pediatric, Short Term

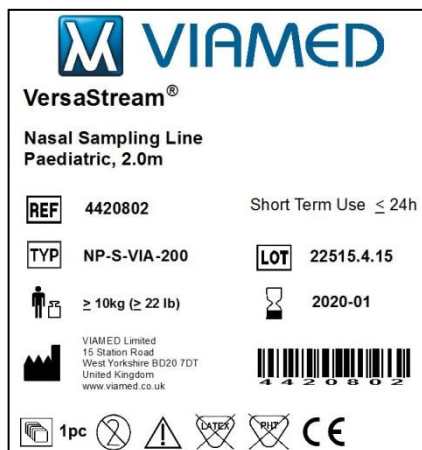


Front view

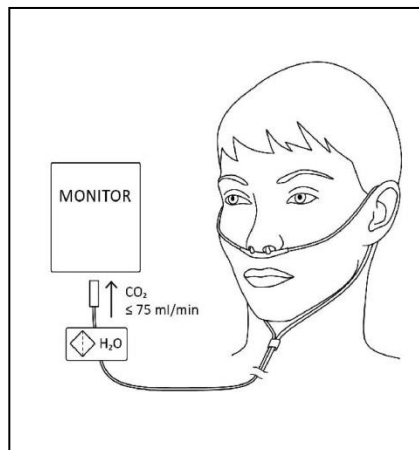

Rear view


Box Label

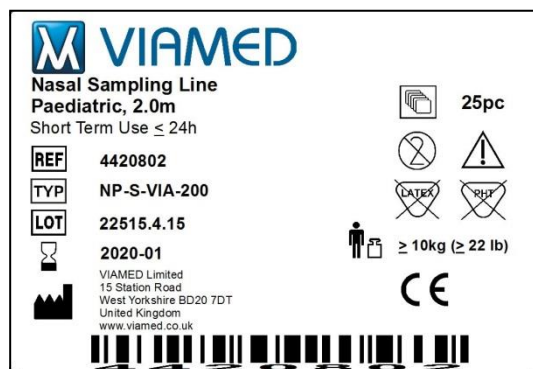


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 5 von 29

Ref.: 4420803, Typ: NI-S-VIA-200
Nasal Sampling Line, Infant, Short Term

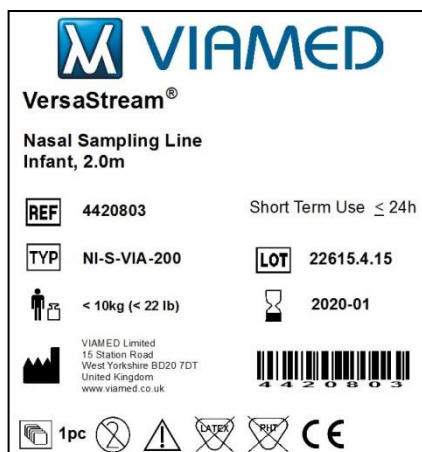


Front view

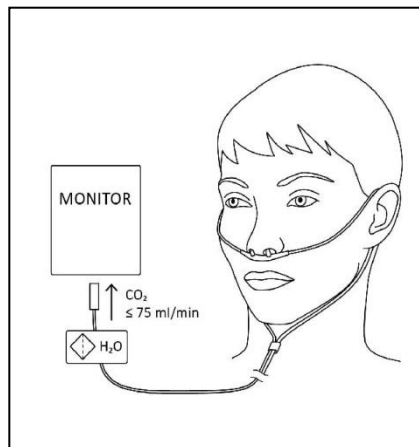

Rear view


Box Label

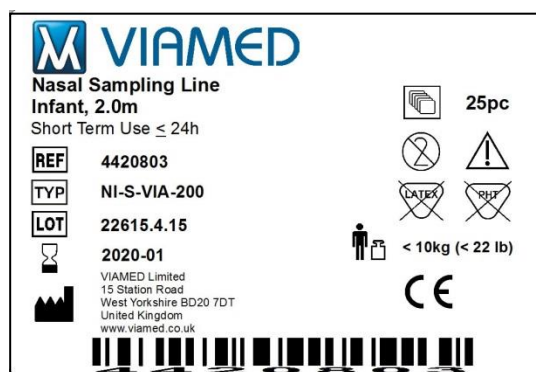


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 6 von 29

Ref.: 4420804, Typ: NAO2-S-VIA-200
Nasal Sampling Line with O2 Supply, Adult, Short Term

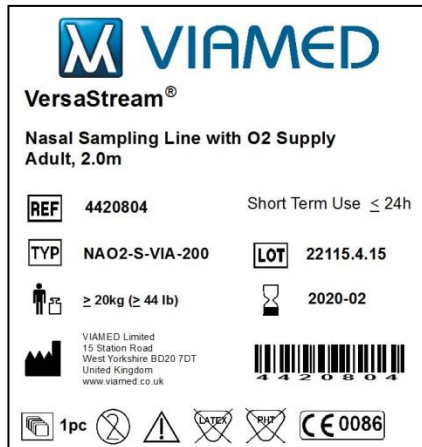


Front view

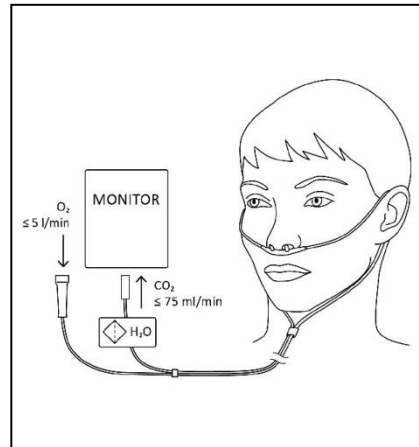

Rear view


Box Label

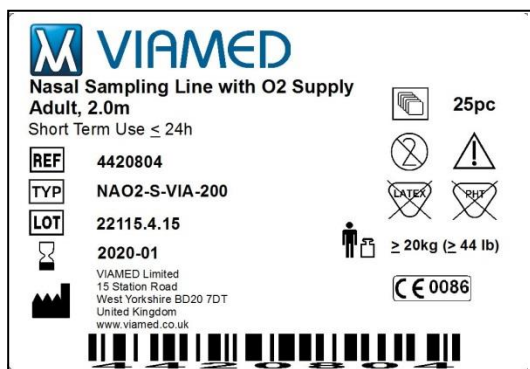


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 7 von 29

Ref.: 4420805, Typ: NPO2-S-VIA-200
Nasal Sampling Line with O2 Supply, Pediatric, Short Term

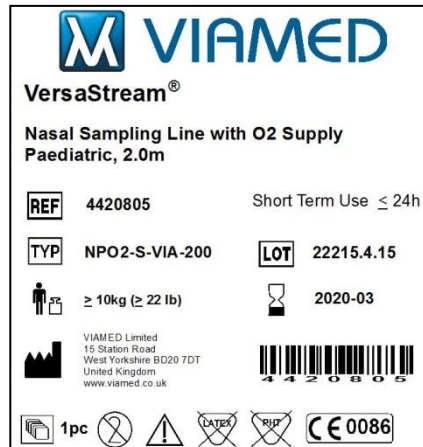


Front view

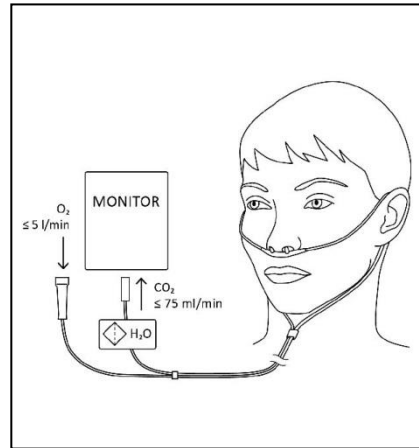

Rear view

Box Label

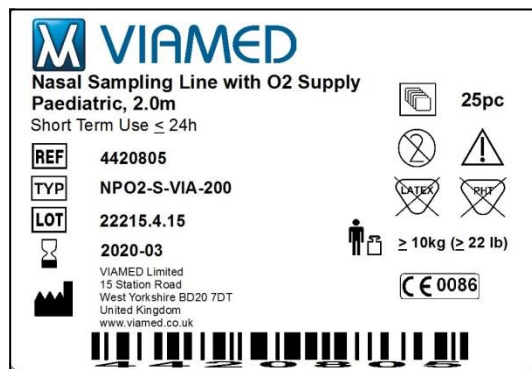

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 9 von 29

Ref.: 4420807, Typ: NA-L-VIA-200
Nasal Sampling Line, Adult, Long Term

Is identical with Ref.: 4420801, Typ: NA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420808, Typ: NP-L-VIA-200
Nasal Sampling Line, Pediatric, Long Term

Is identical with Ref.: 4420802, Typ: NP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420809, Typ: NI-L-VIA-200
Nasal Sampling Line, Infant, Long Term

Is identical with Ref.: 4420803, Typ: NI-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420810, Typ: NAO2-L-VIA-200
Nasal Sampling Line with O2 Supply, Adult, Long Term

Is identical with Ref.: 4420804, Typ: NAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420811, Typ: NPO2-L-VIA-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term

Is identical with Ref.: 4420805, Typ: NPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420812, Typ: NIO2-L-VIA-200
Nasal Sampling Line with O2 Supply, Infant, Long Term

Is identical with Ref.: 4420806, Typ: NIO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 10 von 29

Ref.: 4420813, Typ: ONA-S-VIA-200
Oral/Nasal Sampling Line, Adult, Short Term




Front view

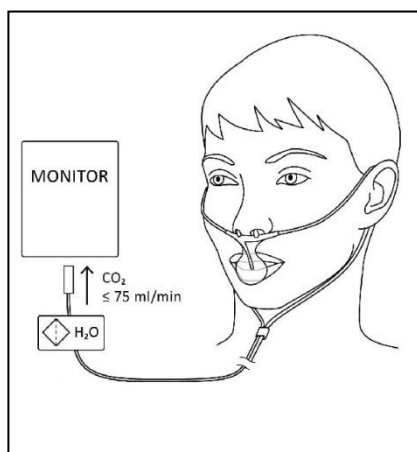

Rear view


Box Label

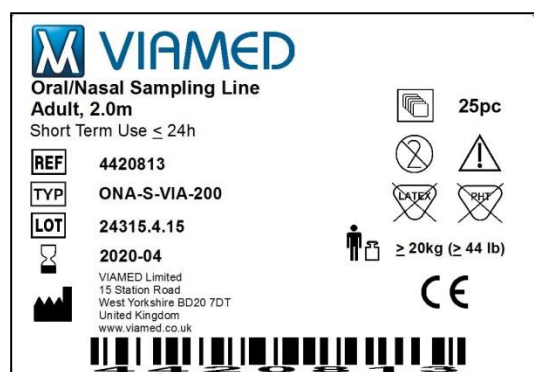


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 11 von 29

Ref.: 4420814, Typ: ONP-S-VIA-200
Oral/Nasal Sampling Line, Paediatric, Short Term

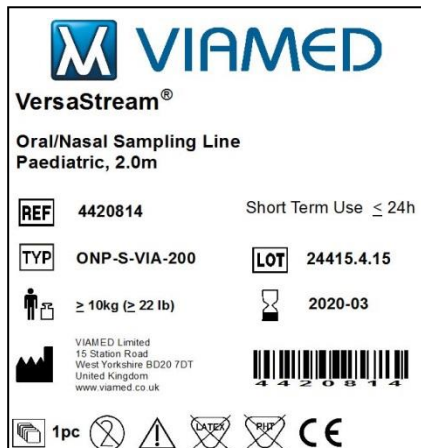


Front view

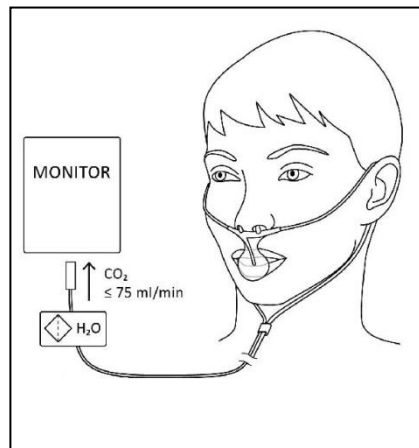

Rear view


Box Label

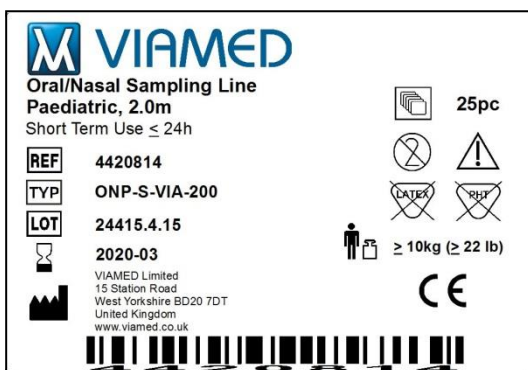


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 12 von 29

Ref.: 4420815, Typ: ONAO2-S-VIA-200
 Oral/Nasal Sampling Line with O2 Supply, Adult, Short Term

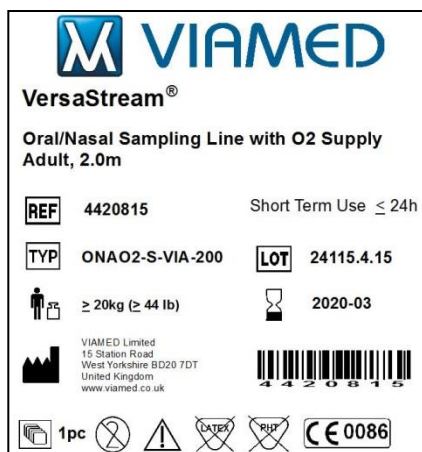


Front view

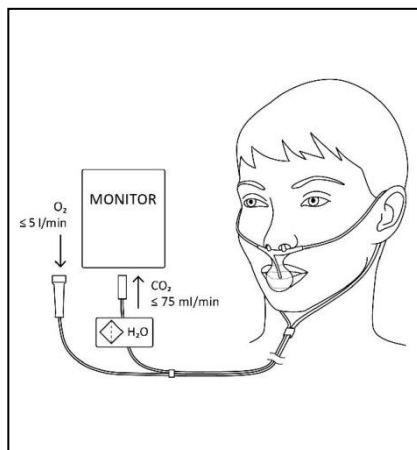

Rear view


Box Label

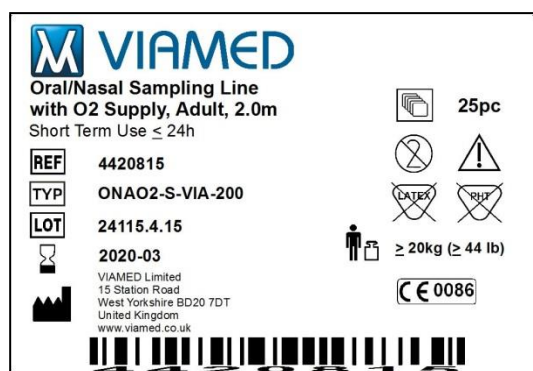


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 13 von 29

Ref.: 4420816, Typ: ONPO2-S-VIA-200
Oral/Nasal Sampling Line with O2 Supply, Pediatric, Short Term

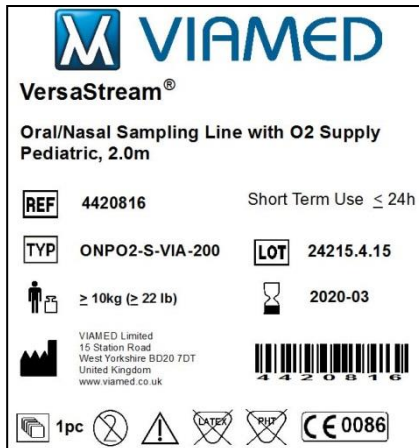


Front view

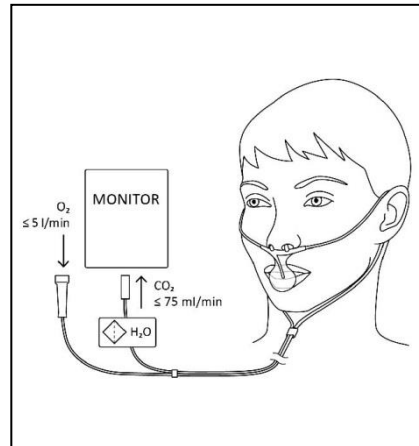

Rear view

Box Label

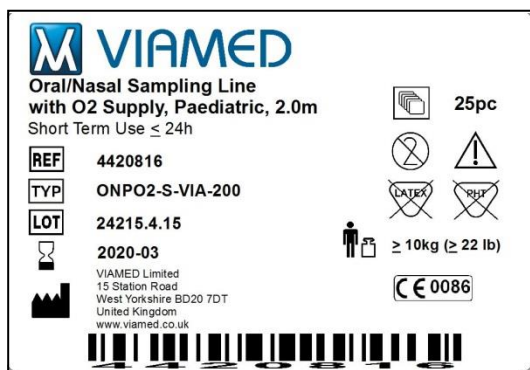

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 14 von 29

**Ref.: 4420817, Typ: ONA-L-VIA-200
Nasal Sampling Line, Adult, Long Term**

**Is identical with Ref.: 4420813, Typ: ONA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420818, Typ: ONP-L-VIA-200
Nasal Sampling Line, Pediatric, Long Term**

**Is identical with Ref.: 4420814, Typ: ONP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420819, Typ: ONAO2-L-VIA-200
Nasal Sampling Line with O2 Supply, Adult, Long Term**

**Is identical with Ref.: 4420815, Typ: ONAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**


**Ref.: 4420820, Typ: ONPO2-L-VIA-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term**

**Is identical with Ref.: 4420816, Typ: ONPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 16 von 29

Ref.: 4420822, Typ: A4.0-S-VIA-200
Airway Adapter Sampling Line, Infant, Short Term

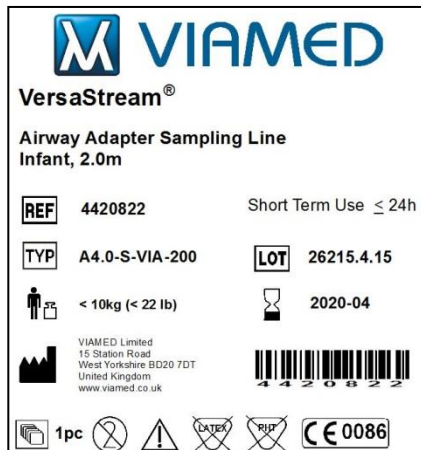


Front view

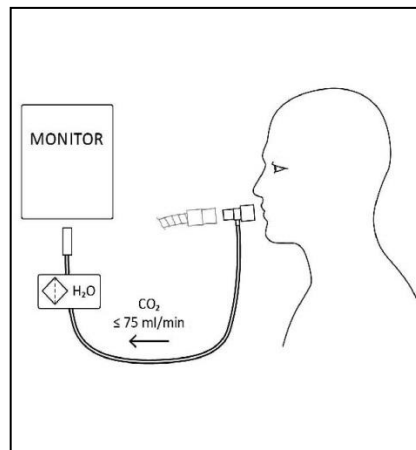

Rear view

Box Label

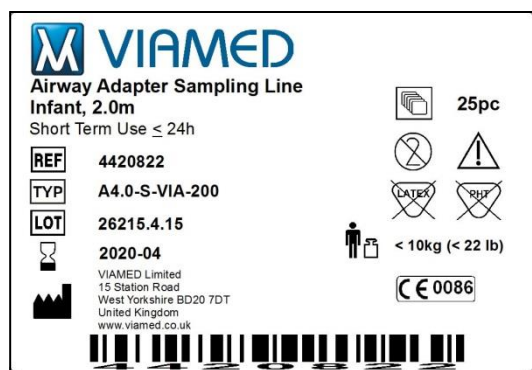

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 17 von 29

Ref.: 4420823, Typ: A22-L-VIA-200

Airway Adapter Sampling Line, Adult/Pediatric, Long Term

Is identical with Ref.: 4420821, Typ: A22-S-VIA-200

Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420824, Typ: A4.0-L-VIA-200

Airway Adapter Sampling Line, Infant, Long Term

Is identical with Ref.: 4420822, Typ: A4.0-S-VIA-200

Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 18 von 29

2. Label Layout: LLM Connector Sampling Lines

Ref.: 4420850, Typ: P-S-LLM-200
Single Port Nasal Prong, Adult, Short Term

Is identical with Ref.: 4420800, Typ: P-S-VIA-200

Ref.: 4420851, Typ: NA-S-LLM-200
Nasal Sampling Line, Adult, Short Term

Is identical with Ref.: 4420801, Typ: NA-S-VIA-200

Ref.: 4420852, Typ: NP-S-LLM-200
Nasal Sampling Line, Pediatric, Short Term

Is identical with Ref.: 4420802, Typ: NP-S-VIA-200

Ref.: 4420853, Typ: NI-S-LLM-200
Nasal Sampling Line, Infant, Short Term

Is identical with Ref.: 4420803, Typ: NI-S-VIA-200

Ref.: 4420854, Typ: NAO2-S-LLM-200
Nasal Sampling Line with O2 Supply, Adult, Short Term

Is identical with Ref.: 4420804, Typ: NAO2-S-VIA-200

Ref.: 4420855, Typ: NPO2-S-LLM-200
Nasal Sampling Line with O2 Supply, Pediatric, Short Term

Is identical with Ref.: 4420805, Typ: NPO2-S-VIA-200

Ref.: 4420856, Typ: NIO2-S-LLM-200
Nasal Sampling Line with O2 Supply, Infant, Short Term

Is identical with Ref.: 4420806, Typ: NIO2-S-VIA-200

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 19 von 29

Ref.: 4420857, Typ: NA-L-LLM-200
Nasal Sampling Line, Adult, Long Term

Is identical with Ref.: 4420801, Typ: NA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420858, Typ: NP-L-LLM-200
Nasal Sampling Line, Pediatric, Long Term

Is identical with Ref.: 4420802, Typ: NP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420859, Typ: NI-L-LLM-200
Nasal Sampling Line, Infant, Long Term

Is identical with Ref.: 4420803, Typ: NI-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420860, Typ: NAO2-L-LLM-200
Nasal Sampling Line with O2 Supply, Adult, Long Term

Is identical with Ref.: 4420804, Typ: NAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420861, Typ: NPO2-L-LLM-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term

Is identical with Ref.: 4420805, Typ: NPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420862, Typ: NIO2-L-LLM-200
Nasal Sampling Line with O2 Supply, Infant, Long Term

Is identical with Ref.: 4420806, Typ: NIO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 20 von 29

Ref.: 4420863, Typ: ONA-S-LLM-200
Oral/Nasal Sampling Line, Adult, Short Term

Is identical with Ref.: 4420813, Typ: ONA-S-VIA-200

Ref.: 4420864, Typ: ONP-S-LLM-200
Oral/Nasal Sampling Line, Pediatric, Short Term

Is identical with Ref.: 4420814, Typ: ONP-S-VIA-200

Ref.: 4420865, Typ: ONAO2-S-LLM-200
Oral/Nasal Sampling Line with O2 Supply, Adult, Short Term

Is identical with Ref.: 4420815, Typ: ONAO2-S-VIA-200

Ref.: 4420866, Typ: ONPO2-S-LLM-200
Oral/Nasal Sampling Line with O2 Supply, Pediatric, Short Term

Is identical with Ref.: 4420816, Typ: ONPO2-S-VIA-200

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 21 von 29

**Ref.: 4420867, Typ: ONA-L-LLM-200
Nasal Sampling Line, Adult, Long Term**

**Is identical with Ref.: 4420813, Typ: ONA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420868, Typ: ONP-L-LLM-200
Nasal Sampling Line, Pediatric, Long Term**

**Is identical with Ref.: 4420814, Typ: ONP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420869, Typ: ONAO2-L-LLM-200
Nasal Sampling Line with O2 Supply, Adult, Long Term**

**Is identical with Ref.: 4420815, Typ: ONAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420870, Typ: ONPO2-L-LLM-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term**

**Is identical with Ref.: 4420816, Typ: ONPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 22 von 29

Ref.: 4420871, Typ: A22-S-LLM-200
Airway Adapter Sampling Line, Adult/Pediatric, Short Term

Is identical with Ref.: 4420821, Typ: A22-S-VIA-200

Ref.: 4420872, Typ: A4.0-S-LLM-200
Airway Adapter Sampling Line, Infant, Short Term

Is identical with Ref.: 4420822, Typ: A4.0-S-VIA-200

Ref.: 4420873, Typ: A22-L-LLM-200
Airway Adapter Sampling Line, Adult/Pediatric, Long Term

Is identical with Ref.: 4420821, Typ: A22-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Ref.: 4420874, Typ: A4.0-L-LLM-200
Airway Adapter Sampling Line, Infant, Long Term

Is identical with Ref.: 4420822, Typ: A4.0-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 23 von 29

3. Label Layout: RES Connector Sampling Lines

Ref.: 4420950, Typ: P-S-RES-200
Single Port Nasal Prong, Adult, Short Term

Is identical with Ref.: 4420800, Typ: P-S-VIA-200

Ref.: 4420951, Typ: NA-S-RES-200
Nasal Sampling Line, Adult, Short Term

Is identical with Ref.: 4420801, Typ: NA-S-VIA-200

Ref.: 4420952, Typ: NP-S-RES-200
Nasal Sampling Line, Pediatric, Short Term

Is identical with Ref.: 4420802, Typ: NP-S-VIA-200

Ref.: 4420953, Typ: NI-S-RES-200
Nasal Sampling Line, Infant, Short Term

Is identical with Ref.: 4420803, Typ: NI-S-VIA-200

Ref.: 4420954, Typ: NAO2-S-RES-200
Nasal Sampling Line with O2 Supply, Adult, Short Term

Is identical with Ref.: 4420804, Typ: NAO2-S-VIA-200

Ref.: 4420955, Typ: NPO2-S-RES-200
Nasal Sampling Line with O2 Supply, Pediatric, Short Term

Is identical with Ref.: 4420805, Typ: NPO2-S-VIA-200

Ref.: 4420956, Typ: NIO2-S-RES-200
Nasal Sampling Line with O2 Supply, Infant, Short Term

Is identical with Ref.: 4420806, Typ: NIO2-S-VIA-200

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 24 von 29

**Ref.: 4420957, Typ: NA-L-RES-200
Nasal Sampling Line, Adult, Long Term**

**Is identical with Ref.: 4420801, Typ: NA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420958, Typ: NP-L-RES-200
Nasal Sampling Line, Pediatric, Long Term**

**Is identical with Ref.: 4420802, Typ: NP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420959, Typ: NI-L-RES-200
Nasal Sampling Line, Infant, Long Term**

**Is identical with Ref.: 4420803, Typ: NI-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420960, Typ: NAO2-L-RES-200
Nasal Sampling Line with O2 Supply, Adult, Long Term**

**Is identical with Ref.: 4420804, Typ: NAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420961, Typ: NPO2-L-RES-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term**

**Is identical with Ref.: 4420805, Typ: NPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420962, Typ: NIO2-L-RES-200
Nasal Sampling Line with O2 Supply, Infant, Long Term**

**Is identical with Ref.: 4420806, Typ: NIO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 25 von 29

**Ref.: 4420963, Typ: ONA-S-RES-200
Oral/Nasal Sampling Line, Adult, Short Term**

Is identical with Ref.: 4420813, Typ: ONA-S-VIA-200

**Ref.: 4420964, Typ: ONP-S-RES-200
Oral/Nasal Sampling Line, Pediatric, Short Term**

Is identical with Ref.: 4420814, Typ: ONP-S-VIA-200

**Ref.: 4420965, Typ: ONAO2-S-RES-200
Oral/Nasal Sampling Line with O2 Supply, Adult, Short Term**

Is identical with Ref.: 4420815, Typ: ONAO2-S-VIA-200

**Ref.: 4420966, Typ: ONPO2-S-RES-200
Oral/Nasal Sampling Line with O2 Supply, Pediatric, Short Term**

Is identical with Ref.: 4420816, Typ: ONPO2-S-VIA-200

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 26 von 29

**Ref.: 4420967, Typ: ONA-L-RES-200
Nasal Sampling Line, Adult, Long Term**

**Is identical with Ref.: 4420813, Typ: ONA-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420968, Typ: ONP-L-RES-200
Nasal Sampling Line, Pediatric, Long Term**

**Is identical with Ref.: 4420814, Typ: ONP-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420969, Typ: ONAO2-L-RES-200
Nasal Sampling Line with O2 Supply, Adult, Long Term**

**Is identical with Ref.: 4420815, Typ: ONAO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

**Ref.: 4420970, Typ: ONPO2-L-RES-200
Nasal Sampling Line with O2 Supply, Pediatric, Long Term**

**Is identical with Ref.: 4420816, Typ: ONPO2-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h**

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 27 von 29

Ref.: 4420971, Typ: A22-S-RES-200
Airway Adapter Sampling Line, Adult/Pediatric, Short Term

Is identical with Ref.: 4420821, Typ: A22-S-VIA-200

Ref.: 4420972, Typ: A4.0-S-RES-200
Airway Adapter Sampling Line, Infant, Short Term

Is identical with Ref.: 4420822, Typ: A4.0-S-VIA-200

Ref.: 4420973, Typ: A22-L-RES-200
Airway Adapter Sampling Line, Adult/Pediatric, Long Term

Is identical with Ref.: 4420821, Typ: A22-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h


Ref.: 4420974, Typ: A4.0-L-RES-200
Airway Adapter Sampling Line, Infant, Long Term

Is identical with Ref.: 4420822, Typ: A4.0-S-VIA-200
Only Change: Short Term Use $\leq$ 24h → Long Term Use $\leq$ 72h


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R.Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 28 von 29

Ref.: 4420975, Typ: LLM-S-RES-200
Luer Lock Sampling Line, Short Term

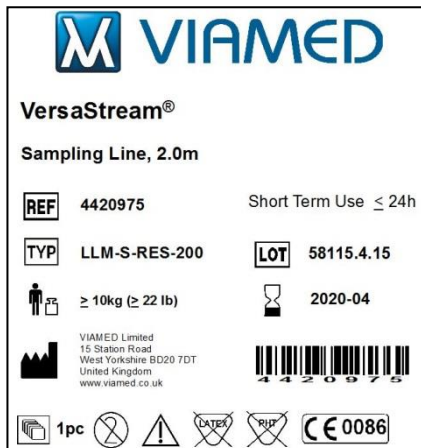


Front view

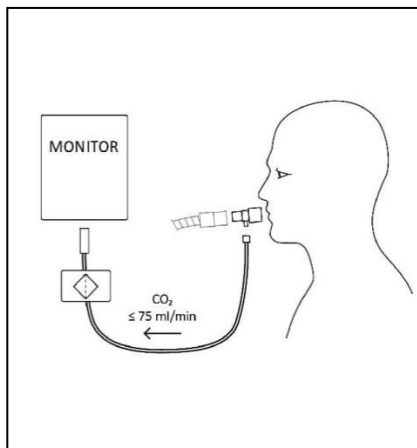

Rear view

Box Label

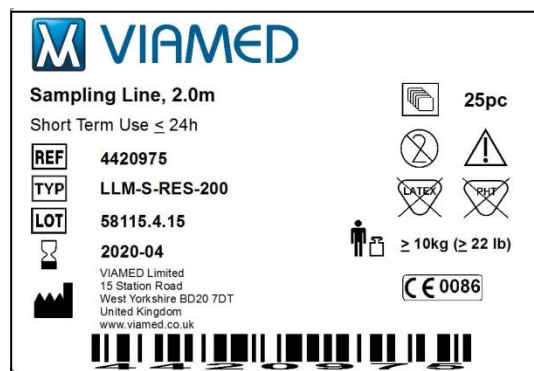


Ref.: 4420976, Typ: LLM-L-RES-200
Luer Lock Sampling Line, Long Term

Is identical with Ref.: 4420875, Typ: LLM-S-RES-200
Only Change: Short Term Use ≤ 24h → Long Term Use ≤ 72h


Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	

bluepoint MEDICAL	PHA VersaStream Sampling Lines	Revision 0
Internal Document	4.9 Viamed Labeling OEM	Seite 29 von 29

Tag Layout:

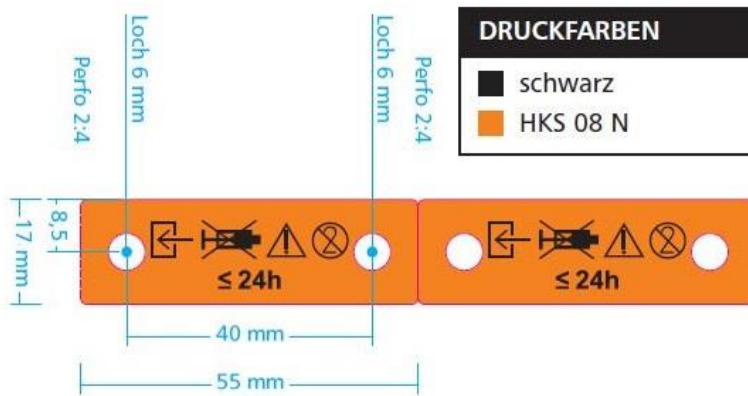

Tag for short term sampling lines

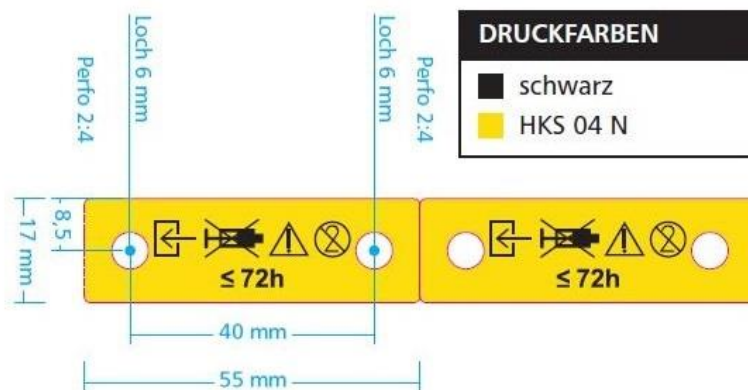

Tag for long term sampling lines

Erstellt: R. Jürgensen Datum: 2015-04-13	Freigabe: R. Jürgensen Datum: 2015-04-13
Datei: 4.9_Labeling_OEM_rev0	