

List of Private Label



Customer: VIAMED



Confidential!

Only for use by EnviteC and VIAMED!

Contents

1	List of Sensors	2
2	Änderungsregister / Change log	2
3	R- 23V (OOM201)	3
4	R- 30V (OOM110)	3
5	R- 41V (OOM202-1)	3
6	R- 42V (OOM202-2S).....	4
7	R- 43V (OOM112)	4
8	R- 44V (OOM202-2)	4
9	R- 45V (OOM106)	5
10	R- 46V (OOM111).....	5
11	R-47V (OOM204).....	5
12	R-49V (OOM202).....	6
13	R- 22MEDV (OOM103).....	6
14	R- 48V (OOM113).....	6
15	Customer Approval	7

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	1 / 7

List of Private Label



Customer: VIAMED



Confidential!

Only for use by EnviteC and VIAMED!

1 List of Sensors

No.	EnviteC Sensor - Type	Viamed PN = EnviteC Order Ref.	Envitec Article number	Final model number
1	OOM201	0110023	01-00-0014	R- 23V
2	OOM110	0110040	01-00-0098	R- 30V
3	OOM202-1	0110041	01-00-0021	R- 41V
4	OOM202-2S	0110042	1000106	R- 42V
5	OOM112	0110043	1001202	R- 43V
6	OOM202-2	0110044	01-00-0068	R- 44V
7	OOM106	0110045	01-00-0091	R- 45V
8	OOM111	0110046	01-00-0114	R- 46V
9	OOM204	0110047	01-00-0097	R- 47V
10	OOM202	0110049	01-00-0047	R- 49V
11	OOM103	0110021	01-00-0015	R- 22MEDV
12	OOM113	0110048	1002178	R-48V

2 Änderungsregister / Change log

Revision	Date	Author	Description
0	10.12.2014	Maik Lingies	New document design data from document "Private Label VIAMED_update_2013-07-16" and add the Sensor type OOM202, OOM204 and OOM113

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	2 / 7

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

Only for use by EnviteC and VIAMED!

3 R- 23V (OOM201)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor Class R- 23V CE 0086 Part No. 0110023 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT SN V 12345 E 10	MEDICAL OXYGEN SENSOR Class R- 23V CE 0086 Part No. 0110023 SN V 12345 E 10 2010-05 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk
4 R- 30V (OOM110)	
Label on Sensor (dia. 39,8)	Label on Blister- Card (63,5x46,6)
VIAMED Medical Oxygen Sensor CE 0086 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • UK www.viamed.co.uk SN V 12345 E 10 Part No. 0110040 Class R- 30V CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT	MEDICAL OXYGEN SENSOR Class R- 30V CE 0086 Part No. 0110040 SN V 12345 E 10 2010-05 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk
5 R- 41V (OOM202-1)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor Class R- 41V CE 0086 Part No. 0110041 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT SN V 12345 E 10	MEDICAL OXYGEN SENSOR Class R- 41V CE 0086 Part No. 0110041 SN V 01234 G13 2013-07 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	3 / 7

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

Only for use by EnviteC and VIAMED!

6 R- 42V (OOM202-2S)	
Label on Sensor (90x11)	
Medical Oxygen Sensor CE 0086 SN V 12345 E 10 Class R- 42V Part No. 0110042 CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk	
Label on plastic container (90x11)	
Medical Oxygen Sensor CE 0086 SN V 12345 E 10 Class R- 42V Part No. 0110042 CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk	
7 R- 43V (OOM112)	
Label on Sensor (90x15)	Label on single Blister- Card (pack of 2) (63,5x46,6)
Medical Oxygen Sensor CE 0086 SN V 12345 E 10 Class R- 43V Part No. 0110043 CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk	MEDICAL OXYGEN SENSOR Class R- 43V CE 0086 Part No. 0110043 SN V 12345 E 10 2010-05 NON-STERILE! Do not remove the sensor from the packaging until ready to use! 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk
8 R- 44V (OOM202-2)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor CE 0086 SN V 12345 E 10 Class R- 44V Part No. 0110044 CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk	MEDICAL OXYGEN SENSOR Class R- 44V CE 0086 Part No. 0110044 SN V 12345 E 10 2010-05 NON-STERILE! Do not remove the sensor from the packaging until ready to use! 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	4 / 7

List of Private Label


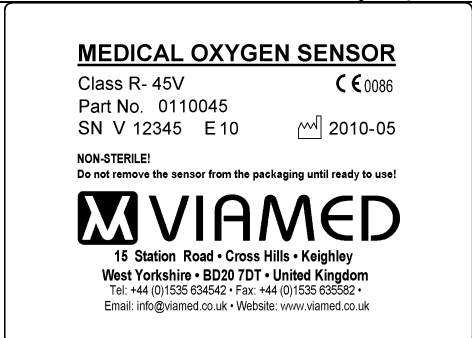

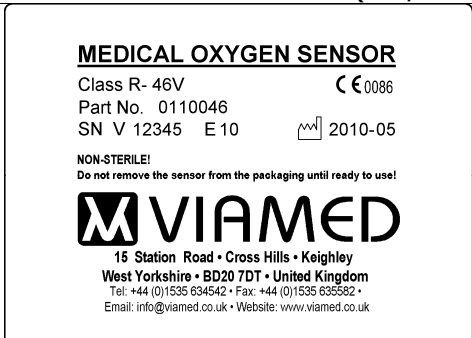

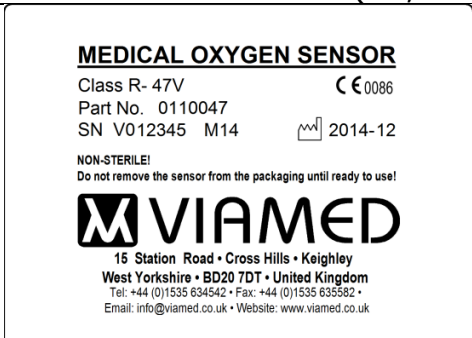
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

Only for use by EnviteC and VIAMED!

9 R- 45V (OOM106)	
Label on Sensor (90x11) 	Label on Blister- Card (63,5x46,6) 
10 R- 46V (OOM111)	
Label on Sensor (90x15) 	Label on Blister- Card (63,5x46,6) 
11 R-47V (OOM204)	
Label on Sensor (90x15) 	Label on Blister- Card (63,5x46,6) 

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	5 / 7

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

Only for use by EnviteC and VIAMED!

12 R-49V (OOM202)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor CE 0086 SN V012345 M14 Class R- 49V Part No. 0110049 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT	MEDICAL OXYGEN SENSOR Class R- 49V CE 0086 Part No. 0110049 SN V012345 M14 2014-12 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk
13 R- 22MEDV (OOM103)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor CE 0086 SN V01234 G13 Class R-22MEDV Part No. 0110021 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT	MEDICAL OXYGEN SENSOR Class R-22MEDV CE 0086 Part No. 0110021 SN V01234 G13 2013-07 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk
14 R- 48V (OOM113)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
Medical Oxygen Sensor CE 0086 SN V012345 M14 Class R- 48V Part No. 0110048 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Fax: +44 (0)1535 635582 Email: info@viamed.co.uk Website: www.viamed.co.uk CONTAINS CAUSTIC SUBSTANCE EXCEEDS 0.4% LEAD BY WEIGHT	MEDICAL OXYGEN SENSOR Class R- 48V CE 0086 Part No. 0110048 SN V012345 M14 2014-12 NON-STERILE! Do not remove the sensor from the packaging until ready to use! VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 • Fax: +44 (0)1535 635582 • Email: info@viamed.co.uk • Website: www.viamed.co.uk

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	6 / 7

List of Private Label

Customer: VIAMED

Confidential!

Only for use by EnviteC and VIAMED!

Honeywell

ENVITEC

by Honeywell

15 Customer Approval

Date:

Signature:

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigabe n\001-29-Private_Label_VIAMED-0.docx	ML 6/24/2015	7 / 7