


Orantech

The **difference** you can **sense**

CE 0123

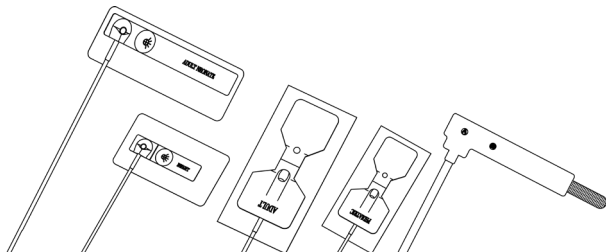

Single-patient-use SpO₂ Sensors

User Manual

Intended Use & Indications for Use

The SpO₂ sensors are intended for continuous noninvasive monitoring of functional oxygen saturation of arterial hemoglobin (SpO₂) and pulse rate (PR).

These compatible replacement sensors are intended for use with major pulse oximeter brands. The SpO₂ sensors are designed to match the specifications of the original equipment manufacturer, therefore confirm that the appropriate sensor model numbers are being used with the correct pulse oximeter technology.

The sensors are available for the following patient sizes:

- Adult (weight greater than 40 kg)
- Pediatric (10-50 kg weight)
- Infant (3-20 kg weight)
- Neonate (weight less than 3 kg)

Contraindication

The probe should not be fixed at the site of tissue damage, and should not be used for blood oxygen monitoring in hyperactive patients.

Principle of Operation


The sensors must be connected to its corresponding monitor. Blood oxygenation is measured by detecting the infrared and red light absorption characteristics of deoxygenated hemoglobin and oxygenated hemoglobin, which consists of a probe attached to the patient. The sensor is connected to a data acquisition system which is used to calculate and display oxygen saturation levels and heart rate conditions.

Installation

- Connect the SpO₂ sensor to the oximeter's adapter cable.
- Turn the oximeter on and verify proper operation.
- Select the sensor site on the patient. The preferred sensor sites are the index finger for adult and

children, the great toe for infants, and on the foot below the toes for neonate.

- Place the sensor on the patient.

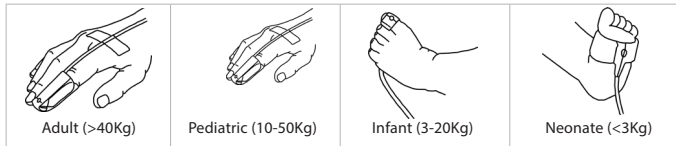

- Position the emitter and detector directly opposite each other.
- Visually monitor the sensor site to ensure that over time there is no harm to the patient's skin.

Caution

- ⚠ Place the sensor on the index finger ensuring the finger is fully inserted and the tip of the finger rests against the finger stop inside the sensor.
- ⚠ Possible alternate sites are small-sized thumb, middle and ring fingers as well as the little finger or the big toe.
- ⚠ Ensure the fingernail is located under the finger stop on the SpO₂ sensor clamp.
- ⚠ The sensor must not be located on the same arm as the blood pressure cuff, arterial catheter or intravascular line.
- ⚠ Remove all nail polish as this can affect accuracy.
- ⚠ Do not use the sensor inside or near an MRI.
- ⚠ Avoid intense light sources near the sensor.
- ⚠ The sensor site must be inspected at least every eight (8) hours; and if the circulatory condition or skin integrity has changed, the sensor should be applied to a different site.
- ⚠ The site must be checked frequently or per clinical protocol to ensure adequate adhesion, circulation, skin integrity and correct optical alignment.
- ⚠ Exercise caution with poorly perfused patients; skin erosion and pressure necrosis can be caused when the sensor is not frequently moved. Assess site as frequently as every (1) hour with poorly

perfused, patients and move the sensor if there are signs of tissue ischemia.

- ⚠️ Circulation distal to the sensor site should be checked routinely
- ⚠️ During low perfusion, the sensor site needs to be assessed frequently for signs of tissue ischemia, which can lead to pressure necrosis.

Equipment

- Connect the sensor adapter cable to the appropriate equipment (or pulse oximeter).
- Turn on the equipment and check correct operation by consulting the monitor's operation instructions.
- To ensure proper monitor operations, connect and disconnect the sensor cable from the monitor cable. The correct, safe use of the sensor and its connecting cable requires systematic checks to be carried out at least once or more per month depending on the frequency of use, as well as disinfecting the cable.
- Do a visual check (appearance of insulators, connector contact pins, etc.).
- Verify the mechanical integrity of the connectors.

Do not use and discard any sensor that appears to have any mechanical or electrical flaws.

Performance, Reliability, Safety, Compatibility & Mechanical Integrity

• Performance/Reliability

This SpO₂ sensor with its compatible pulse oximeter has been validated and tested for compliance with ISO 80601-2-61.

Comparative value measurement in % saturation:

SpO₂ range (70%-100%) -Accuracy $\pm 3\%$

SpO₂ range (<70%) -No specified

Pulse rate range: 35-240 bpm -Accuracy ± 2 bpm

Low perfusion: SpO₂ range (70%-100%) -Accuracy $\pm 3\%$

Pulse rate range: 35-240 bpm -Accuracy ± 3 bpm

- **Peak Wavelength and Maximum Output Power**

LED Type	RED Peak Wavelength	RED Maximum Output Power	IR Peak Wavelength	IR Maximum Output Power
2-Leads	663 nm	1.2 mW	890 nm	1.0 mW
3-Leads	661 nm	1.2 mW	940 nm	1.2 mW
4-Leads	660 nm	1.2 mW	905/940 nm	1.0 mW

- **Safety**

Degree of protection from electric shocks: type BF

Classification is in accordance with MDD 93/42/EEC: Class IIb

Degree of protection against the Ingress of Water: IPX1

- **Compatibility**

In order to ensure compatibility and claimed accuracy of the devices, the SpO₂ sensor should only be used with the specified equipment for which they have been designed and labeled for use.

- **Mechanical Integrity**

This sensor is designed to be extremely durable. We use only the highest quality materials to ensure the sensors stand up to the demanding hospital environment. The solid connectors are fitted with flexible sleeves to minimize the risk of cable breakage. They have no accessible metallic parts.

Operating Conditions

- Ambient temperature: 0°C to +40°C
- Relative humidity: 15% to 85%
- Atmospheric pressure: 86 kpa ~ 106 kpa

Storage & Packaging

Each sensor is individually packaged.

Sensors must be stored in its original packaging and within the storage conditions to maximize the storage life.

Storage conditions are as follows:


- Ambient temperature: -10°C to +40°C
- Relative humidity: 15% to 85%
- Atmospheric pressure: 86 kpa ~ 106 kpa










Shelf Life

2 years.








Warning

 The sensors should not be fixed in the tissue injury site, not for hyperactivity of blood oxygen monitoring.

-  The sensors are designed for use with specific monitors.
-  The operator is responsible for checking the compatibility of the monitor, sensor and cable before its use.
-  Incompatible components can result in degraded accuracy and performance.
-  Consult the operation instructions for the equipment concerned and the related accessories before operating equipment to ensure their compatibility.
-  Portable and mobile RF communications equipment can be affect equipment.
-  Do not immerse connector ends in cleaning solution(s).
-  Do not allow service or maintenance on the sensor while used on a patient.
-  No modification of this sensor is allowed.
-  The sensors are tested by biocompatibility, there are not any risk to the human body.

Warning: MR Unsafe!

-  Do not expose the device to a magnetic resonance (MR) environment.
-  The device may present a risk of projectile injury due to the presence of ferromagnetic materials that can be attracted by the MR magnet core.
-  Thermal injury and burns may occur due to the metal components of the device that can heat during MR scanning.
-  The device may generate artifacts in the MR image.
-  The device may not function properly due to the strong magnetic and radiofrequency fields generated by the MR scanner.




















Caution

 Federal (U.S.) Law restricts this device to sale by or on the order of a physician.

Waste Disposal









Please refer to your local laws and regulations for information on how to dispose of SpO₂ sensors.

Title of Symbol

	Manufacturer		Warning
	Catalogue number		Caution
	Batch code		Date of manufacture
	Serial number		Crossed out wheellie bin indicates separate treatment from general waste at end of life. Waste of Electrical and Electronic Equipment Directive (WEEE)
	Not made with natural rubber latex		Authorized Representative in the European Community
	Refer to instruction manual /booklet		CE Mark
	Non-sterile		Type BF Applied Part
Rx only(U.S.)	Federal (U.S.) Law restricts this device to sale by or on the order of a physician		Medical device
	Protection against vertically falling water drops		Unique Device Identifier
	Single patient use		
	Use-by date		

Support

To get the support, please contact the representative of manufacturer or local distributor.
The categories shown below are available for sale through the local distributors or e-commerce.

			
SpO₂	ECG	NIBP	IBP
			
TEMP	EtCO₂	FETAL	EEG



Orantech Inc.

Zone#A, 4F, 1st Bld, 7th Industrial Zone, Yulv Community, GongMing,
Guangming New District, Shenzhen, China 518106

☎ www.orantech.com ☎ (+86) 755 2369 9939 ☎ info@orantech.com

Medten EU Aps

Hejreskovvej 8, 3490 Kvistgård, Denmark

REF: M20-M008

Rev: A3