

List of Private Label

Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

1 / 11

List of Private Label

Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

1 List of Sensors

No.	EnviteC Sensor - Type	Viamed PN = EnviteC Order Ref.	Envitec Article number	Final model number
1	OOM201	0110023	01-00-0014	R- 23V
2	OOM110	0110040	01-00-0098	R- 30V
3	OOM202-1	0110041	01-00-0021	R- 41V
4	OOM202-2S	0110042	1000106	R- 42V
5	OOM112	0110043	1001202	R- 43V
6	OOM202-2	0110044	01-00-0068	R- 44V
7	OOM106	0110045	01-00-0091	R- 45V
8	OOM111	0110046	01-00-0114	R- 46V
9	OOM204	0110047	01-00-0097	R- 47V
10	OOM202	0110049	01-00-0047	R- 49V
11	OOM103	0110021	01-00-0015	R- 22MEDV
12	OOM113	0110048	1002178	R-48V

2 Änderungsregister / Change log

Revision	Date	Author	Description
0	10.12.2014	Maik Lingies	New document design data from document "Private Label VIAMED_update_2013-07-16" and add the Sensor type OOM202, OOM204 and OOM113



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

2 / 11

List of Private Label

Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

3 R- 23V (OOM201)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
VIAMED Medical Oxygen Sensor TYPE: R- 23V SN: Z123456 2015-09	Medical Oxygen Sensor TYPE R- 23V PN 0110023 SN Z123456 2015-09 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C
4 R- 30V (OOM110)	
Label on Sensor (dia. 39,8)	Label on Blister- Card (63,5x46,6)
VIAMED Medical Oxygen Sensor TYPE: R- 30V SN: Z123456 2015-09	Medical Oxygen Sensor TYPE R- 30V PN 0110040 SN Z123456 2015-09 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C
5 R- 41V (OOM202-1)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

3 / 11

List of Private Label

Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

VIAMED Tel: +44 (0)1535 534542 Email: info@viamed.co.uk Website: www.viamed.co.uk Medical Oxygen Sensor TYPE: R-41V S/N: Z123456   0086   2015-09	Medical Oxygen Sensor TYPE R-41V PN 0110041 SN  Z123456       2015-09 VIAMED  0086 15 Station Road • Cross Hills • Kelghley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1535 534542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
--	---



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

4 / 11

List of Private Label




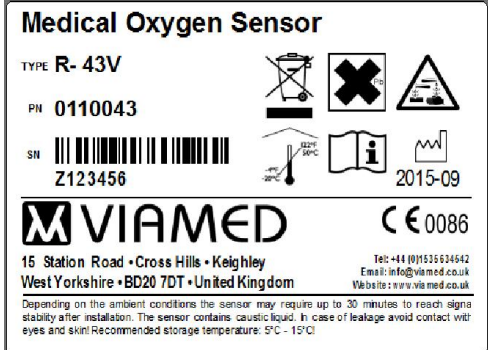
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

6 R- 42V (OOM202-2S)	
Label on Sensor (90x11)	
	
Label on plastic container (90x11)	
	
7 R- 43V (OOM112)	
Label on Sensor (90x15)	Label on single Blister- Card (pack of 2) (63,5x46,6)
	



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

5 / 11

List of Private Label


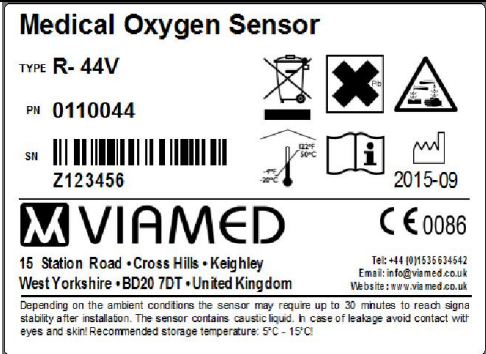
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

8 R- 44V (OOM202-2)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
	



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

6 / 11

List of Private Label


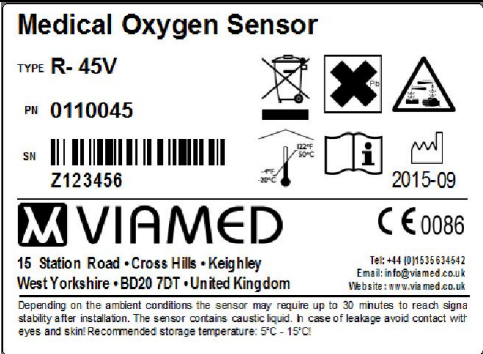
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

9 R- 45V (OOM106)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
	
10 R- 46V (OOM111)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

7 / 11

List of Private Label


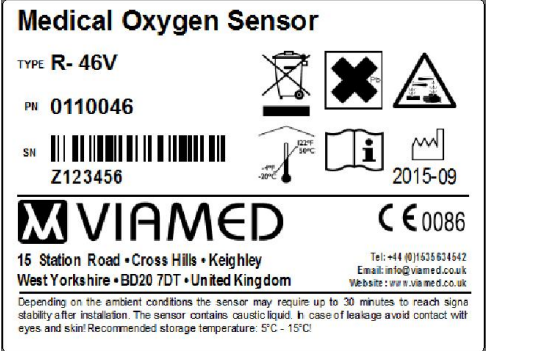

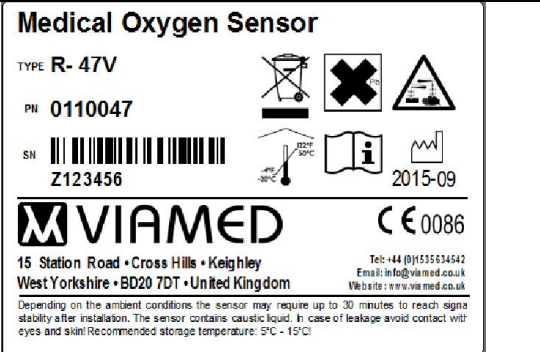
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

	
11 R-47V (OOM204)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

8 / 11

List of Private Label


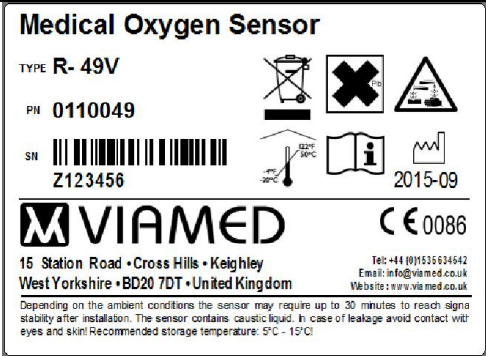
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

12 R-49V (OOM202)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
13 R- 22MEDV (OOM103)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

9 / 11

List of Private Label


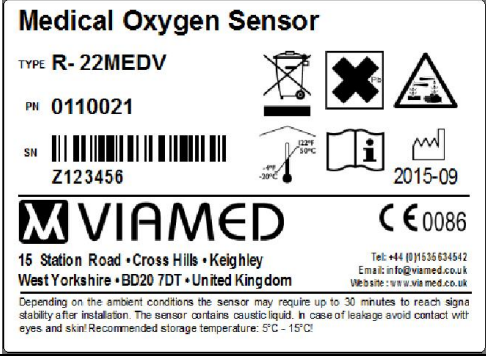

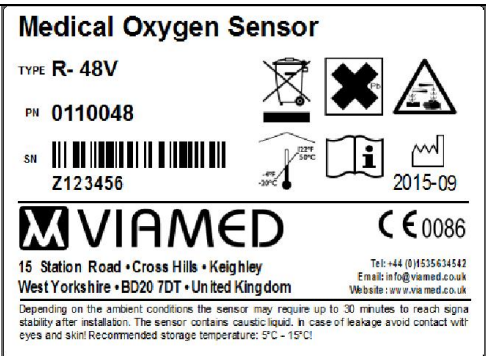
Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

	
14 R- 48V (OOM113)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	

15 Customer Approval



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

10 / 11

List of Private Label

Customer: VIAMED

Confidential!

For use by EnviteC and VIAMED only!

Honeywell

ENVITEC
by Honeywell

Date:

Signature:



Created –
Erstellt:
Page –
Seite:

T:\Derek Lamb\001-29-Private_Label_VIAMED-1.doc

9/29/2015

11 / 11