


DESIGN YOUR OWN PHOTO-THERAPAY LIGHT SHIELD & OXYGEN HOOD

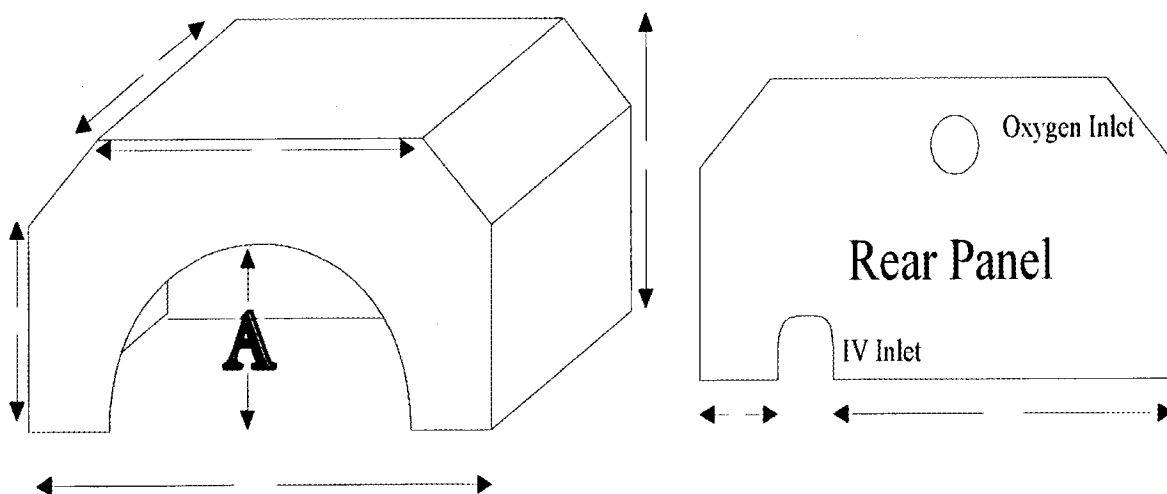

Please insert the dimensions that you require (in mm)

Indicate the Position & Size of:

- O₂ Inlet Holes (normally 22mm)
- IV Line Slots
- Extra Holes
- Side Ports
- Temperature Probe (if required) (18mm hole)
- Flow Diverter (if required) (18mm hole)

Following our standard design style would be preferred, but other designs may be possible.

Please complete the following:

<p>Do you require?</p> <p>Soft front flap (available for neck openings up to a maximum arc length of 330mm) <input type="checkbox"/></p> <p>Adjustable sliding front <input type="checkbox"/></p> <p>If yes, what is the maximum height of the point?</p> <p>A when closed? <input type="text"/></p> <p>Temperature Probe <input type="text"/></p> <p>Flow Diverter? <input type="text"/></p> <p>Clear Perspex <input type="text"/></p> <p>Or</p> <p>Amber 300 Perspex <input type="text"/></p> <p>(for use with phototherapy)</p>	<p>Name:</p> <p>Department:</p> <p>Hospital:</p> <p>Telephone No:</p> <p>Signature:</p> <p>Date:</p>
--	---