


### DESIGN YOUR OWN OXYGEN HOOD

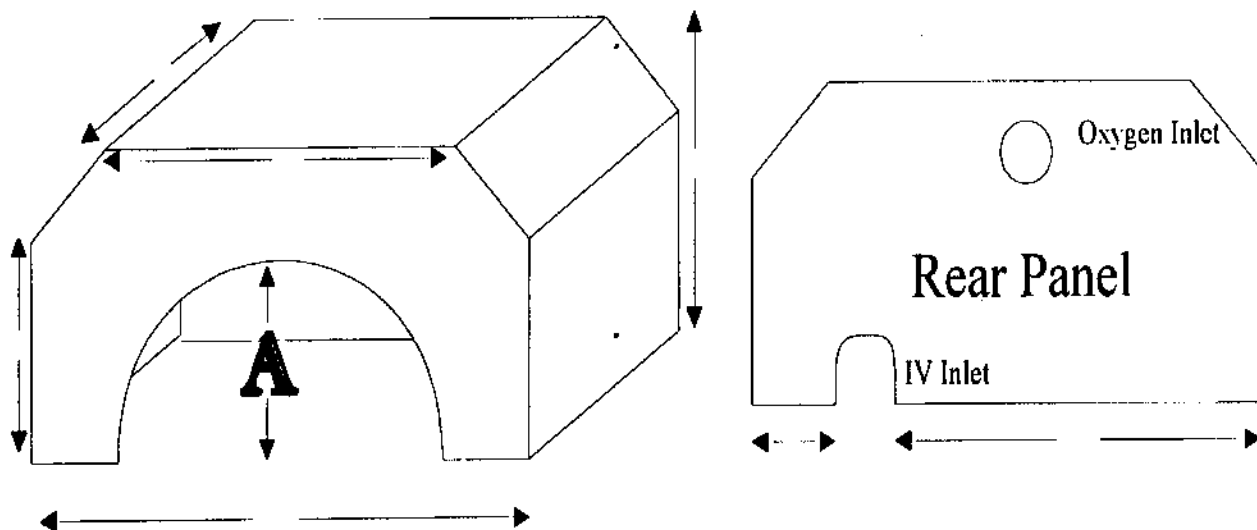

Please insert the dimensions that you require (in mm)

#### Indicate the Position & Size of:

- O<sub>2</sub> Inlet Holes (normally 22mm)
- IV Line Slots
- Extra Holes
- Side Ports
- Temperature Probe (if required) (18mm hole)
- Flow Diverter (if required) (18mm hole)

Following our standard design style would be preferred, but other designs may be possible.

#### Please complete the following:

<p><b>Do you require?</b></p> <p>Soft front flap (available for neck openings up to a maximum arc length of 330mm) <input type="checkbox"/></p> <p>Adjustable sliding front <input type="checkbox"/></p> <p>If yes, what is the maximum height of the point?</p> <p><b>A</b> when closed? <input type="text"/></p> <p>Temperature Probe <input type="text"/></p> <p>Flow Diverter? <input type="text"/></p> <p>Clear Perspex <input type="text"/></p> <p>Or</p> <p>Amber 300 Perspex <input type="text"/></p> <p>(for use with phototherapy)</p>	<p>Name: _____</p> <p>Department: _____</p> <p>Hospital: _____</p> <p>Telephone No: _____</p> <p>Signature: _____</p> <p>Date: _____</p>
--	---