

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

Contents

1	List of Sensors	2
2	Änderungsregister / Change log	2
3	R- 23V (OOM201)	3
4	R- 30V (OOM110)	3
5	R- 41V (OOM202-1)	4
6	R- 42V (OOM202-2S).....	4
7	R- 43V (OOM112)	5
8	R- 44V (OOM202-2)	5
9	R- 45V (OOM106)	6
10	R- 46V (OOM111).....	6
11	R-47V (OOM204).....	7
12	R-49V (OOM202).....	7
13	R- 22MEDV (OOM103).....	8
14	R- 48V (OOM113).....	8
15	R- 15V (OOM101).....	9
16	Customer Approval	9

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	1 / 9

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

1 List of Sensors

No.	EnviteC Sensor - Type	Viamed PN = EnviteC Order Ref.	Envitec Article number	Final model number
1	OOM201	0110023	01-00-0014	R- 23V
2	OOM110	0110040	01-00-0098	R- 30V
3	OOM202-1	0110041	01-00-0021	R- 41V
4	OOM202-2S	0110042	1000106	R- 42V
5	OOM112	0110043	1001202	R- 43V
6	OOM202-2	0110044	01-00-0068	R- 44V
7	OOM106	0110045	01-00-0091	R- 45V
8	OOM111	0110046	01-00-0114	R- 46V
9	OOM204	0110047	01-00-0097	R- 47V
10	OOM202	0110049	01-00-0047	R- 49V
11	OOM103	0110021	01-00-0015	R- 22MEDV
12	OOM113	0110048	1002178	R-48V
13	OOM101	0110014	01-00-0013	R-15V

2 Änderungsregister / Change log

Revision	Date	Author	Description
0	10.12.2014	Maik Lingies	New document design data from document "Private Label VIAMED_update_2013-07-16" and add the Sensor type OOM202, OOM204 and OOM113
1	25.09.2015	Steffen Wickner	Anpassung des Labeldesing nach Anforderungen des DCR550 von Viamed
2	28.10.2015	Steffen Wickner	Change of the Prefix of the serial number from Z to V on request of Viamed
3	14.09.2016	Christian von Walsleben	Change Blister Label accordance to UDI standart
4	06.09.2017	Maik Lingies	Add new Sensor RV-15V

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	2 / 9

List of Private Label


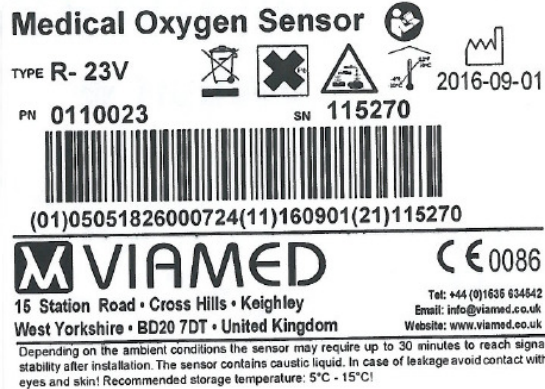
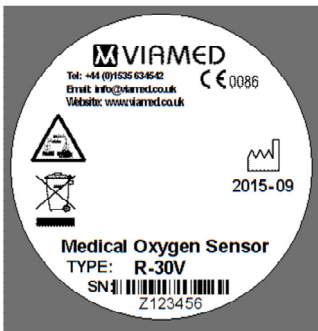
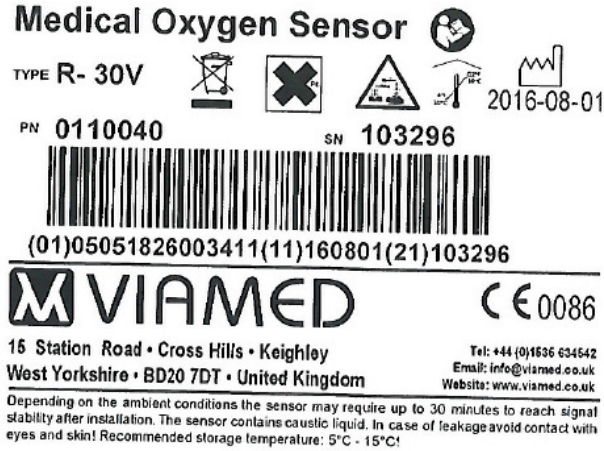
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3 R- 23V (OOM201)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
4 R- 30V (OOM110)	
Label on Sensor (dia. 39,8)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	3 / 9

List of Private Label


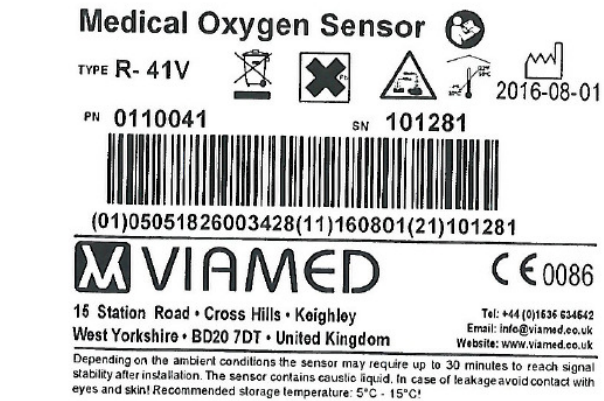


Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

5 R- 41V (OOM202-1)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk CE 0086 TYPE: R- 41V SN: Z123456 2015-09	 Medical Oxygen Sensor TYPE R- 41V PN 0110041 SN 101281 (01)05051826003428(11)160801(21)101281 VIAMED CE 0086 16 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1636 634642 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
6 R- 42V (OOM202-2S)	
Label on Sensor (90x11)	
 VIAMED Medical Oxygen Sensor Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk CE 0086 TYPE: R- 42V SN: Z123456 2015-09	
Label on plastic container (90x11)	
 VIAMED Medical Oxygen Sensor Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk CE 0086 TYPE: R- 42V SN: Z123456 2015-09	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	4 / 9

List of Private Label


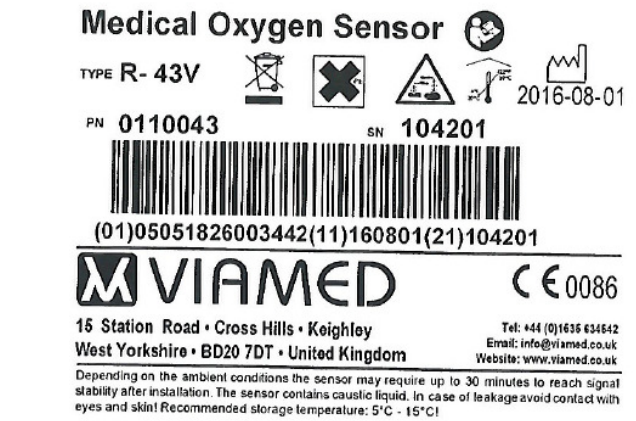

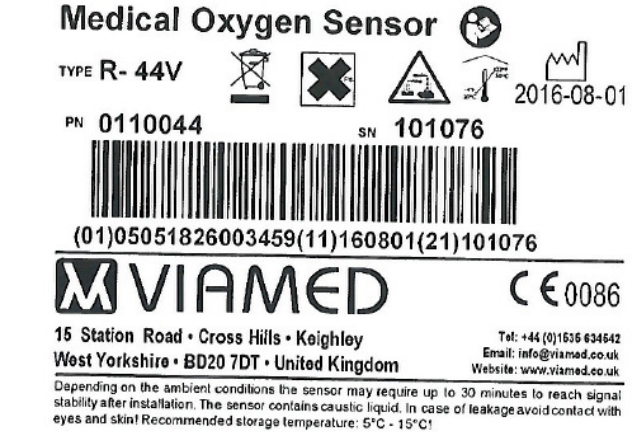
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

7 R- 43V (OOM112)	
Label on Sensor (90x15)	Label on single Blister- Card (pack of 2) (63,5x46,6)
	
8 R- 44V (OOM202-2)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	5 / 9

List of Private Label


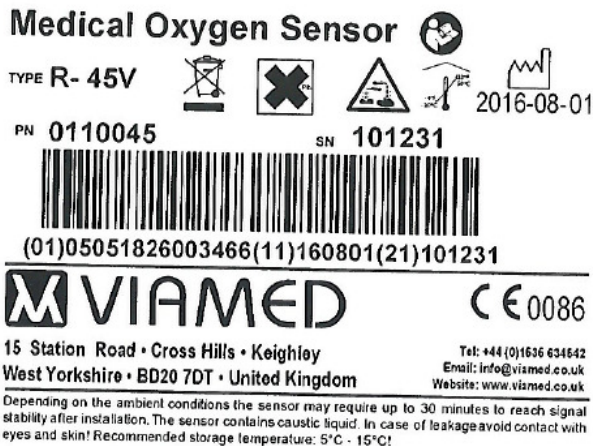

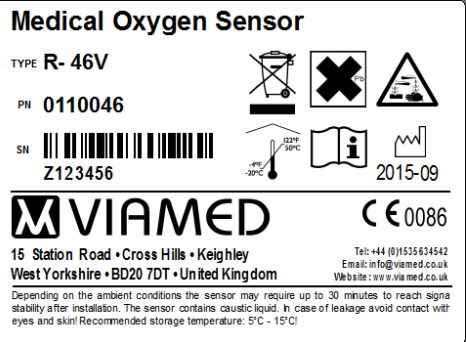
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

9 R- 45V (OOM106)	
Label on Sensor (90x11)	Label on Blister- Card (63,5x46,6)
	
10 R- 46V (OOM111)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	6 / 9

List of Private Label


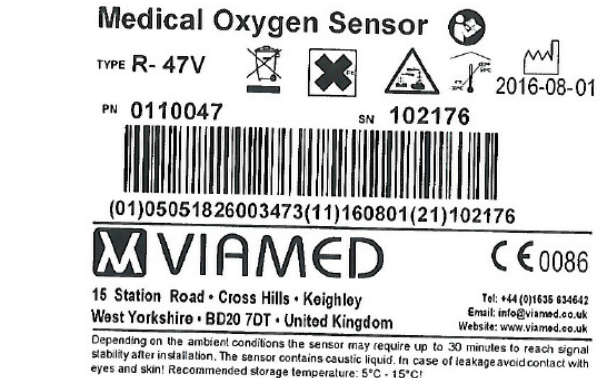

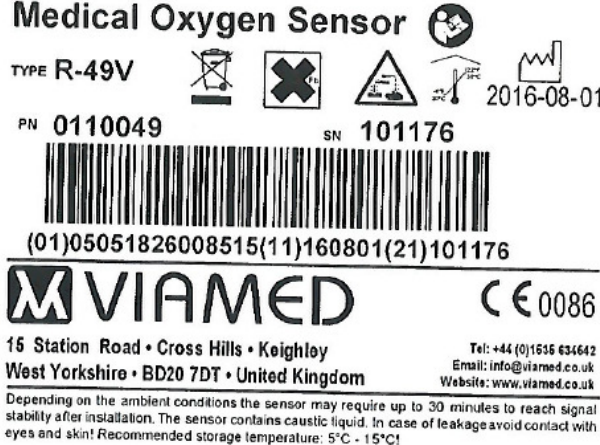
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

11 R-47V (OOM204)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
12 R-49V (OOM202)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	7 / 9

List of Private Label

Honeywell


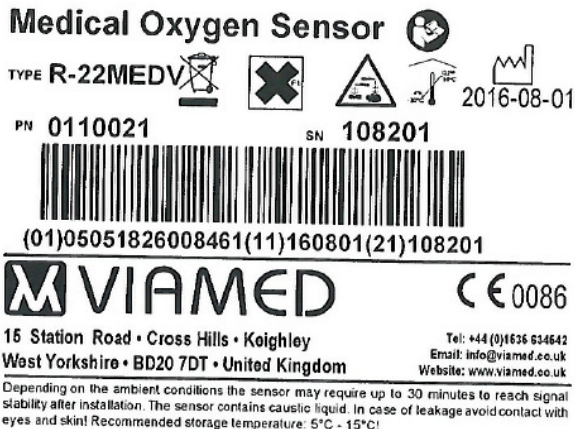

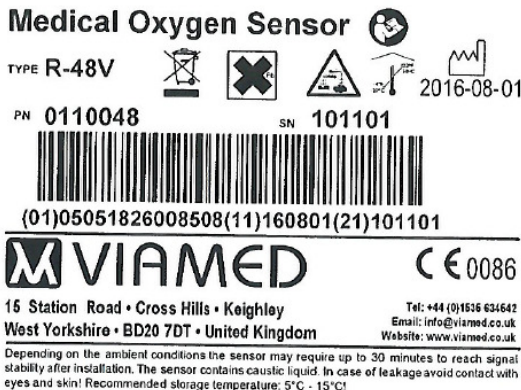
Customer: VIAMED

ENVITEC

by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

13 R- 22MEDV (OOM103)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
14 R- 48V (OOM113)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	8 / 9

List of Private Label


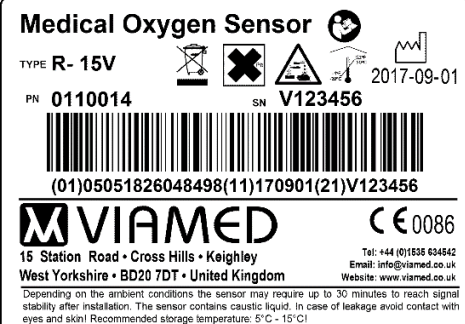
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

15 R- 15V (OOM101)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor TYPE: R- 15V SN: Z123456 2017- 09	 Medical Oxygen Sensor TYPE R- 15V PN 0110014 SN V123456 2017-09-01 (01)05051826048498(11)170901(21)V123456 VIAMED 15 Station Road • Cross Hills • Keighley West Yorkshire • BD20 7DT • United Kingdom Tel: +44 (0)1838 634642 Email: info@viamed.co.uk Website: www.viamed.co.uk CE0086 Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

16 Customer Approval

Date:

Signature:

	Created – Erstellt:	Page – Seite:
\\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx	ML 06.09.2017	9 / 9