


Gas Sampling Line H

en	Instructions for Use
bg	Инструкции за употреба
cs	Návod k použití
da	Brugsanvisning
de	Gebrauchsanweisung
et	Kasutusjuhend
el	Οδηγίες χρήσης
es	Instrucciones de uso
fr	Mode d'emploi
ko	사용 지침
hr	Upute za upotrebu
it	Istruzioni per l'uso
hu	Használati útmutató
nl	Gebruiksaanwijzing
jp	取扱説明書
no	Bruksanvisning
pl	Instrukcja użycia
pt	Instruções de utilização
pt-br	Instruções de uso
ro	Instrucțiuni de utilizare
ru	Инструкция по применению
sl	Navodila za uporabo
sr	Uputstvo za upotrebu
fi	Käyttöohjeet
sv	Bruksanvisning
tr	Kullanım Talimatları
zh	使用说明
ar	إرشادات الاستخدام

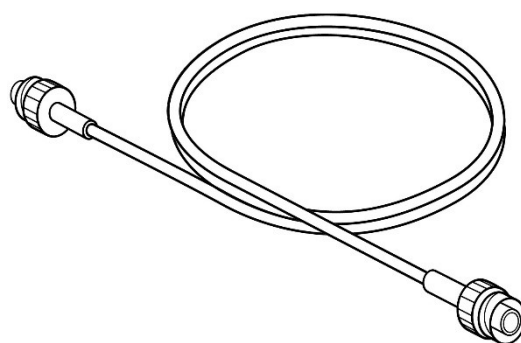

Disposable, 2.5m/8ft

REF 8090121313V

4421517

Intended use

The Gas Sampling Line H is intended for continuous monitoring of expired and inspired respiratory gases. The Gas Sampling Line H is a single patient use device with a cumulative duration of use of up to 24 hours.

The Gas Sampling Line H is for use with the Sedaconda ACD (Anaesthetic Conserving Devices), with adult and pediatric patients, please refer to the Sedaconda ACD Instructions for Use. The Gas Sampling Line H is intended for continuous monitoring of Carbon Dioxide (CO₂), Oxygen (O₂), Sevoflurane, Isoflurane and respiratory rate in professional/hospital care environments, such as operating rooms and intensive care units (ICU).

The Gas Sampling Line H is intended for use by qualified medical personnel only.
Prescription use only.

Warnings

Warning: Only for use with anaesthetic agents Sevoflurane and Isoflurane. Do not use with any other anaesthetic agents.

Warning: Carefully route the sampling line to reduce the risk of patient entanglement or strangulation.

Warning: Do not cut or remove any part of the sampling line. Cutting the sampling line could lead to erroneous readings.

Warning: Due to risk of cross contamination, do not re-use.

Warning: Loose or damaged connections may compromise ventilation or cause an inaccurate measurement of respiratory gases. Securely connect all components and check connections for leaks according to standard clinical procedures.

Warning: Check tubing regularly during use to ensure that no kinks are present. Kinked tubing may cause inaccurate measurement.

Cautions

Caution: Do not attempt to clean, disinfect, sterilize or rinse any part of the sampling line with liquids.

Caution: Dispose of sampling lines in accordance with standard operating procedures or local regulations for the disposal of contaminated medical waste.

Notes

Note: For accuracy specifications and further instructions, warnings and cautions, please consult the gas monitor instructions for use.

Contraindication

There are no known contraindications for patient monitoring with the Airway Gas Sampling Products provided that the data obtained by the gas monitoring is evaluated with consideration given to the patients clinical condition.

Instructions for use

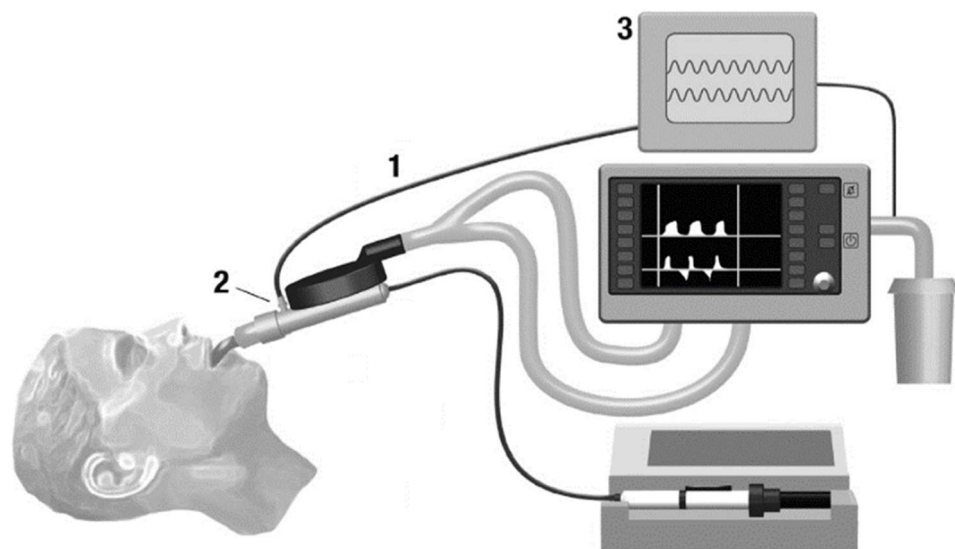


Figure 1

1. Connect the Gas Sampling Line (1) to the Sedaconda ACD gas monitor sampling port (2) as shown in Figure 1. Rotate the Luer connector clockwise for a secure fit to ensure that there is no leakage of gases at the connection point.
2. Connect the Gas Sampling Line (1) to the respiratory gas monitor (3). Rotate the Luer connector clockwise for a secure fit to ensure that there is no leakage of gases at the connection point.
3. After connection of the sampling line, check that gas values appear on the monitor display.

Technical information

Operating temperature: +10 °C to +40 °C (50 °F to 104 °F)
Storage temperature: -25 °C to +60 °C (-13 °F to 140 °F)
Atmospheric pressure: 660 to 1060 hPa (495 to 795 mmHg)
Ambient Humidity: 10 to 95% RH (non-condensing)
For technical specification, see host device user guide or manual.

Reporting of serious incidents

If there is a *serious incident* in connection with the use of this product, this should be reported. The incident should be reported to the manufacturer and the health authority or the competent authority for the installation site of the product. A *serious incident* is when there is a **death or a temporary or permanent serious deterioration in the health of a patient, user or other person**.

Send an email to the following manufacturer address: prrc@bluepoint-medical.com

When doing so, please provide the following information:

- Order number and model designation of the product as indicated on the product
- Serial number/batch number of the product
- Date of the *serious incident*
- Description of the *serious incident*, including its impact on the patient or any injury
- Your contact details (institution, address, contact name (substitute), title and phone number)

Symbols

	Do not reuse
	Not made with natural rubber latex
	Not made with DEHP
	Do not use if package is open or damaged
	Keep dry
	Temperature limitation
	Humidity limitation
	Atmospheric pressure limitation
	Consult instructions for use
	Keep away from sunlight
	CE-Conformité Européene mark
	Medical Device
	Date of manufacture
	Manufacturer
	Catalogue number
	Lot number
	Use by
	Gas inlet
	Do not connect a syringe
	Consult accompanying documents

bg	Инструкции за употреба
cs	Návod k použití
da	Brugsanvisning
de	Gebrauchsanweisung
et	Kasutusjuhend
el	Οδηγίες χρήσης
es	Instrucciones de uso
fr	Mode d'emploi
ko	사용 지침
hr	Upute za upotrebu
it	Istruzioni per l'uso
hu	Használati útmutató
nl	Gebruiksaanwijzing
jp	取扱説明書
no	Bruksanvisning
pl	Instrukcja użycia
pt	Instruções de utilização
pt-br	Instruções de uso
ro	Instrucțiuni de utilizare
ru	Инструкция по применению
sl	Navodila za uporabo
sr	Uputstvo za upotrebu
fi	Käyttöohjeet
sv	Bruksanvisning
tr	Kullanım Talimatları
zh	使用说明
ar	إرشادات الاستخدام



eIFU indicator



IFU Gas Sampling Line H



IFU-06-02-0005 Rev.2 2026-08

Distributed by
Viamed Limited
15 Station Road
Cross Hills, Keighley
West Yorkshire, BD20 7DT
United Kingdom

+44(0)1535 634542
www.viamed.co.uk



bluepoint medical GmbH & Co. KG
An der Trave 15
23923 Selmsdorf
Germany

+49(0)38823 5488 0
www.bluepoint-medical.com