


Quick Start Guide

VM-2105 Silicone Finger Oximeter

This quick start guide details the steps to successfully commence usage of the VM-2105. The full User Instructions can be found on the CD included with the unit*. If you do not have access to a PC, and require a hard copy of these instructions to be sent, please contact Viamed on +44 (0)1535 634542.

Battery Installation

1. Release the lip of the battery compartment on the rear side of the device, in the direction of the arrow. Remove the battery-compartment cover.
2. Insert two batteries (1.5 Volt, AAA), ensuring the correct orientation in accordance with the polarity markings. Ensure that the transparent strips remain accessible once the batteries are inserted.
3. Fold the transparent strips over the batteries and replace the battery-compartment cover, press down until the lip returns to its original position.
4. Depleted batteries can be removed by lightly pulling the transparent strips.

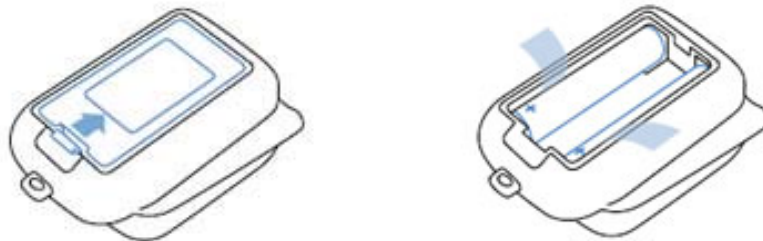


⚠ Externally applied colouring agents, such as nail polish may interfere with the monitor's ability to detect and display accurate measurements!

To obtain an accurate reading it is essential that the finger oximeter is placed correctly on the patient's finger.

The light that is emitted by the finger oximeter has to transmit from the upside of the finger oximeter through the patient's finger nail.

- Turn the patient's hand so that you can see the finger nail.
- Raise the topside of the finger oximeter away from the base slightly, to open.
- Insert the patient's finger, nail facing the top of the finger oximeter, so that the finger is placed fully on the silicone pad.

- Release the topside of the finger oximeter to secure it on to the patient's finger.

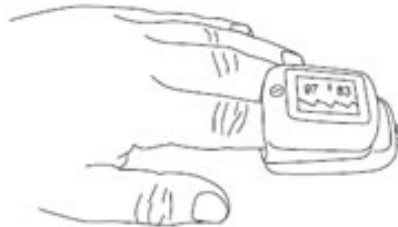


Application and Switching on the Device

Inserting the patient's finger will automatically power on the device, the opening "welcome screen" appears* and then a power-on self-test will initiate.



Self-test in progress.

After the power-on self-test is successfully completed the device will automatically start monitoring.

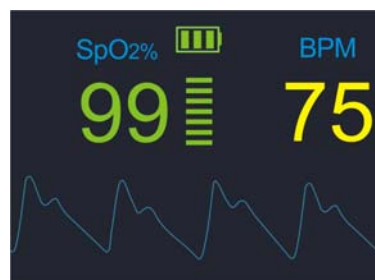

Device in use.

Switching off the Device

The VM-2105 will automatically power off after 15 seconds, when it is removed from the patient's finger.