

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

Contents

1.	List of Sensors	2
2.	Änderungsregister / Change log.....	3
3.	Labelgrafiken / label graphics	4
3.1	R- 23V (OOM201)	4
3.2	R- 30V (OOM110)	4
3.3	R- 41V (OOM202-1)	5
3.4	R- 42V (OOM202-2S)	5
3.5	R- 43V (OOM112)	5
3.6	R- 44V (OOM202-2)	6
3.7	R- 45V (OOM106)	6
3.8	R- 75V (OOM111)	7
3.9	R-47V (OOM204)	7
3.10	R-49V (OOM202)	8
3.11	R- 22MEDV (OOM103)	8
3.12	R- 48V (OOM113)	9
3.13	R- 15V (OOM101)	9
3.14	R-17V (OOM103-1)	10
3.15	R-17Vi (OOM102-1)	10
3.16	R-22Vi (OOM102).....	11
3.17	R-23Vi (OOM104).....	11
3.18	R-22VA (OOM102-A)	12
3.19	T-7V (OOM105)	12
4.	Customer Approval	12

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	1 / 12

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

1. List of Sensors

No.	EnviteC Sensor - Type	Viamed PN = EnviteC Order Ref.	Envitec Article number	Final model number
1	OOM201	0110023	01-00-0014	R- 23V
2	OOM110	0110040	01-00-0098	R- 30V
3	OOM202-1	0110041	01-00-0021	R- 41V
4	OOM202-2S	0110042	1000106	R- 42V
5	OOM112	0110043	1001202	R- 43V
6	OOM202-2	0110044	01-00-0068	R- 44V
7	OOM106	0110045	01-00-0091	R- 45V
8	OOM111	0110075	01-00-0114	R- 75V
9	OOM204	0110047	01-00-0097	R- 47V
10	OOM202	0110049	01-00-0047	R- 49V
11	OOM103	0110021	01-00-0015	R- 22MEDV
12	OOM113	0110048	1002178	R-48V
13	OOM101	0110014	01-00-0013	R-15V
14	OOM103-1	0110018	01-00-0016	R-17V
15	OOM102-1	0110019	01-00-0020	R-17Vi
16	OOM102	0110020	01-00-0019	R-22Vi
17	OOM104	0110025	01-0-0049	R-23Vi
18	OOM102-A	0110039	1002504	R-22VA
19	OOM105	0110058	01-00-0053	T-7V

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	2 / 12

List of Private Label

Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

2. Änderungsregister / Change log

Revision	Date	Author	Description
0	10.12.2014	Maik Lingies	New document design data from document "Private Label VIAMED_update_2013-07-16" and add the Sensor type OOM202, OOM204 and OOM113
1	25.09.2015	Steffen Wickner	Anpassung des Labeldesing nach Anforderungen des DCR550 von Viamed
2	28.10.2015	Steffen Wickner	Change of the Prefix of the serial number from Z to V on request of Viamed
3	14.09.2016	Christian von Walsleben	Change Blister Label accordance to UDI standard
4	06.09.2017	Maik Lingies	Add new Sensor RV-15V
5	16.10.2017	Martin Eckermann	Add new Sensors R-17AG & R-22AG
6	10.12.2018	Maik Lingies	Add new Sensors R-22AVG HAIK
7	26.03.2019	Andrea Ott	Label change for medical sensors according to CE specification. List extended by sensors 3.14 to 3.19. Final model number and Viamed PN for Sensor OOM111 updated.

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Freigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	3 / 12

List of Private Label


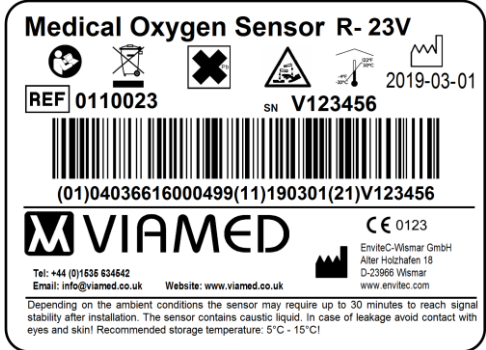
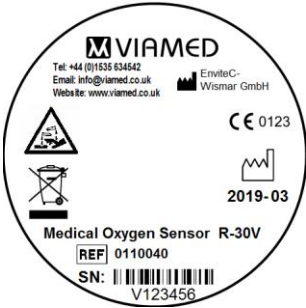
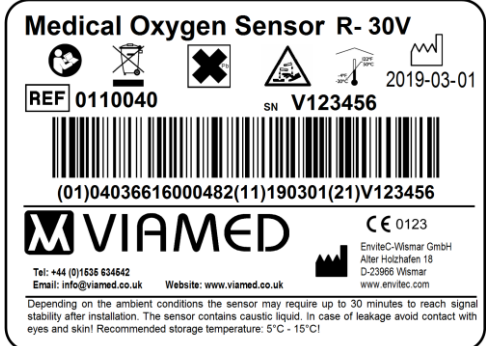
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3. Labelgrafiken / label graphics	
3.1 R- 23V (OOM201)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
3.2 R- 30V (OOM110)	
Label on Sensor (dia. 39,8)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	4 / 12

List of Private Label


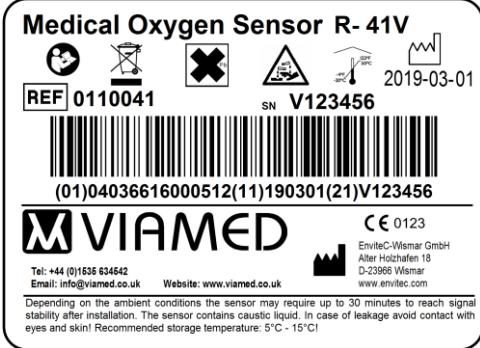


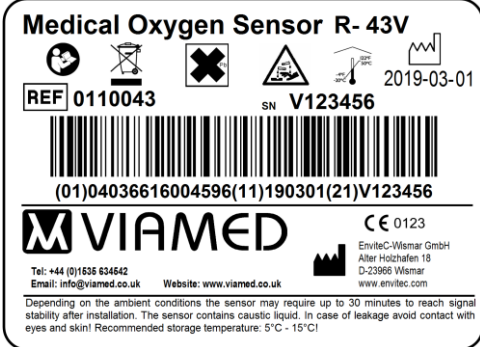
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.3 R- 41V (OOM202-1)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 41V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110041 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 41V REF 0110041 SN V123456 2019-03-01 (01)04036616000512(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.4 R- 42V (OOM202-2S)	
Label on Sensor (90x15)	
 VIAMED Medical Oxygen Sensor R- 42V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110042 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	
Label on plastic container (90x15)	
 VIAMED Medical Oxygen Sensor R- 42V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110042 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	
3.5 R- 43V (OOM112)	
Label on Sensor (90x15)	Label on single Blister- Card (pack of 2) (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 43V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110043 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 43V REF 0110043 SN V123456 2019-03-01 (01)04036616004596(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	5 / 12

List of Private Label


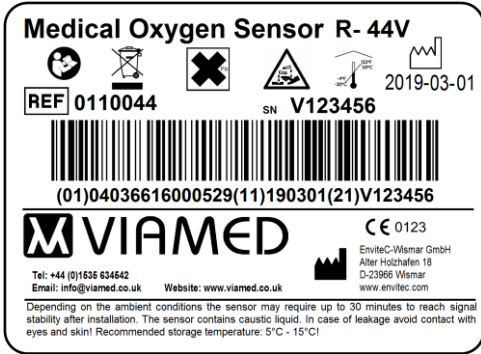

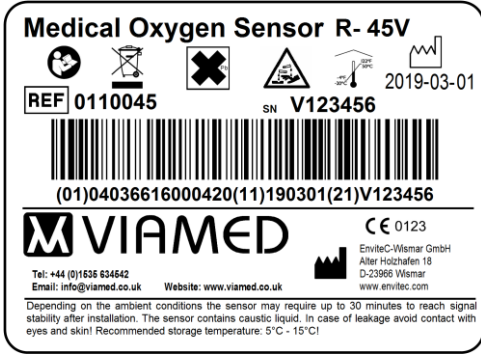
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.6 R- 44V (OOM202-2)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 44V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110044 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 44V REF 0110044 SN V123456 2019-03-01 (01)04036616000529(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.7 R- 45V (OOM106)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 45V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110045 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 45V REF 0110045 SN V123456 2019-03-01 (01)04036616000420(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	6 / 12

List of Private Label


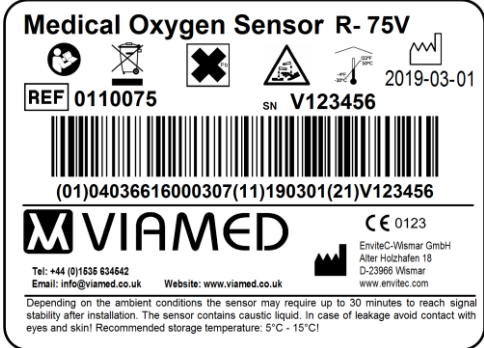
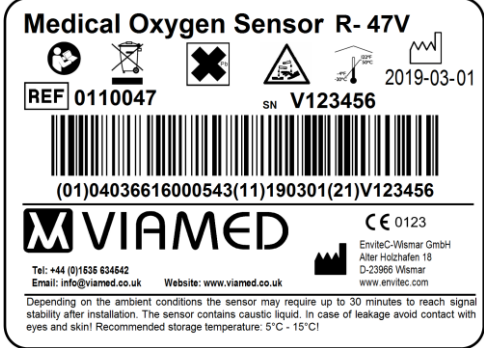
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.8 R- 75V (OOM111)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	
3.9 R-47V (OOM204)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
	

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Freigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	7 / 12

List of Private Label


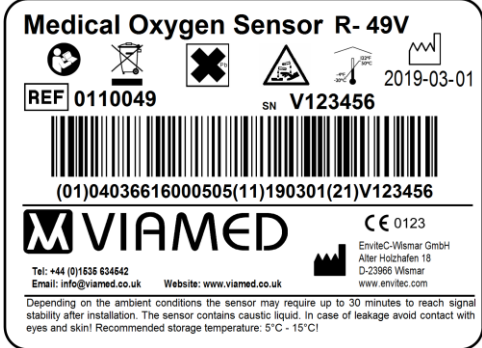

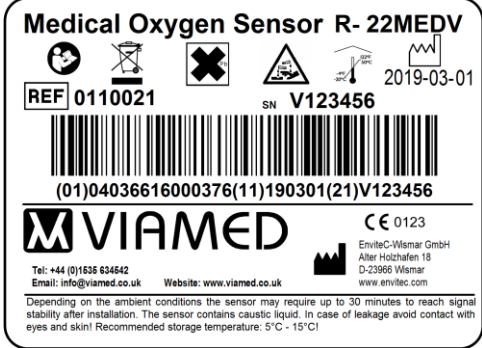
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.10 R-49V (OOM202)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-49V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110049 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-49V REF 0110049 SN V123456 2019-03-01 (01)04036616000505(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhaufen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.11 R- 22MEDV (OOM103)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-22MEDV Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110021 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-22MEDV REF 0110021 SN V123456 2019-03-01 (01)04036616000376(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhaufen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navision\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	8 / 12

List of Private Label

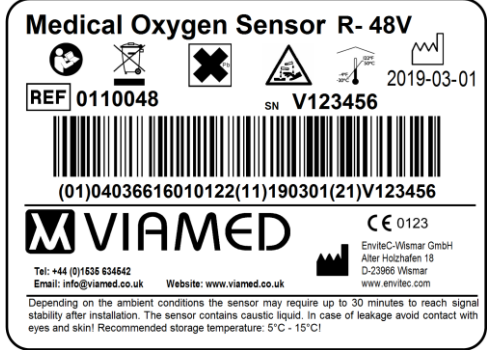
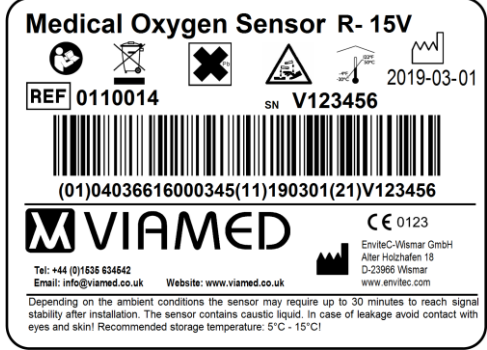
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.12 R- 48V (OOM113)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 48V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110048 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 48V REF 0110048 SN V123456 2019-03-01 (01)04036616010122(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.13 R- 15V (OOM101)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R- 15V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110014 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R- 15V REF 0110014 SN V123456 2019-03-01 (01)04036616000345(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	9 / 12

List of Private Label

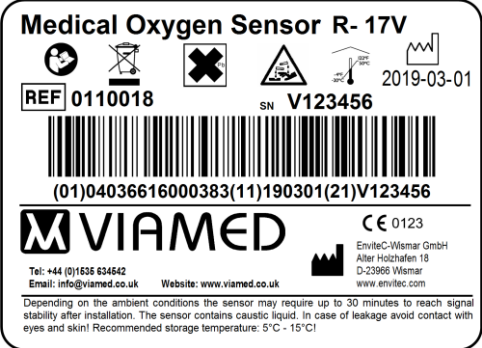
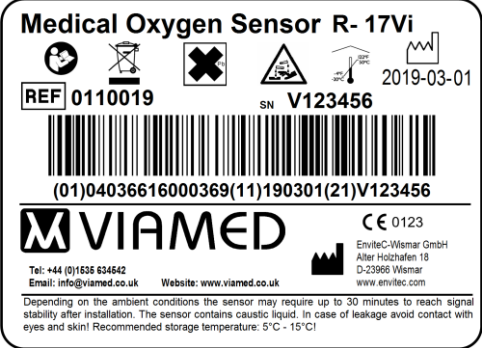
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.14 R-17V (OOM103-1)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-17V REF 0110018 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-17V REF 0110018 SN V123456 2019-03-01 (01)04036616000383(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1635 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.15 R-17Vi (OOM102-1)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-17Vi REF 0110019 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-17Vi REF 0110019 SN V123456 2019-03-01 (01)04036616000369(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1635 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	10 / 12

List of Private Label


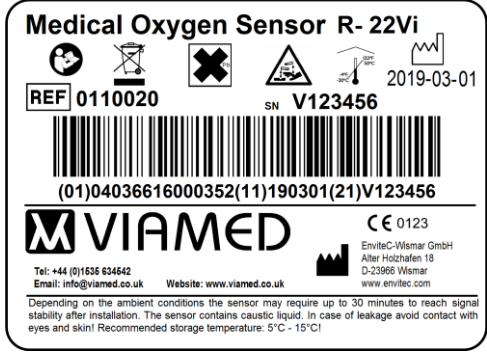
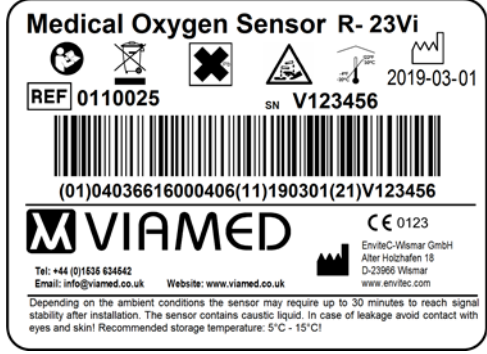
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.16 R-22Vi (OOM102)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-22Vi Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110020 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-22Vi REF 0110020 SN V123456 2019-03-01 (01)04036616000352(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.17 R-23Vi (OOM104)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-23Vi Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110025 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-23Vi REF 0110025 SN V123456 2019-03-01 (01)04036616000406(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	11 / 12

List of Private Label

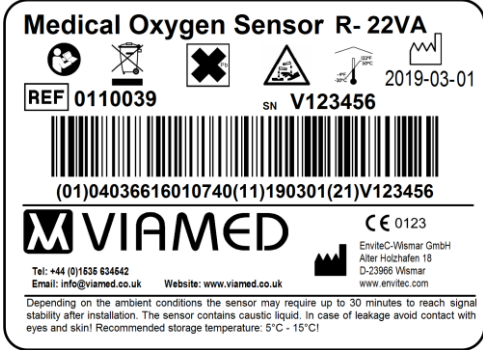
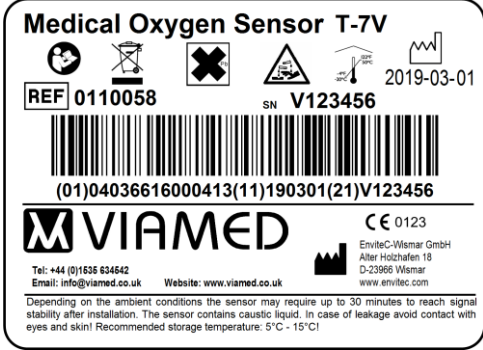
Honeywell

Customer: VIAMED

ENVITEC
by Honeywell

Confidential!

For use by EnviteC and VIAMED only!

3.18 R-22VA (OOM102-A)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor R-22VA Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110039 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor R-22VA REF 0110039 SN V123456 2019-03-01 (01)04036616010740(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!
3.19 T-7V (OOM105)	
Label on Sensor (90x15)	Label on Blister- Card (63,5x46,6)
 VIAMED Medical Oxygen Sensor T-7V Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk REF 0110058 SN: V123456 EnviteC-Wismar GmbH CE 0123 2019-03	 Medical Oxygen Sensor T-7V REF 0110058 SN V123456 2019-03-01 (01)04036616000413(11)190301(21)V123456 VIAMED CE 0123 EnviteC-Wismar GmbH Alter Holzhafen 18 D-23966 Wismar www.envitec.com Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

4. Customer Approval

Date:

Signature:

	Created – Erstellt:	Page – Seite:
R:\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Fr eigaben\001-29-Private_Label_VIAMED-7.docx	AH 28.03.2019	12 / 12