


Date: 31st March 2005

	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
OPEN	0	0.1	0.2	0.4	0.7	1.1	1.5	1.8	2.1	2.8	3.8	4.3	4.7	5.5	6
CLOSED	1.6	1.8	2	2.3	2.5	2.9	3.2	3.5	3.9	4.3	5	5.4	5.8	6.3	6.6

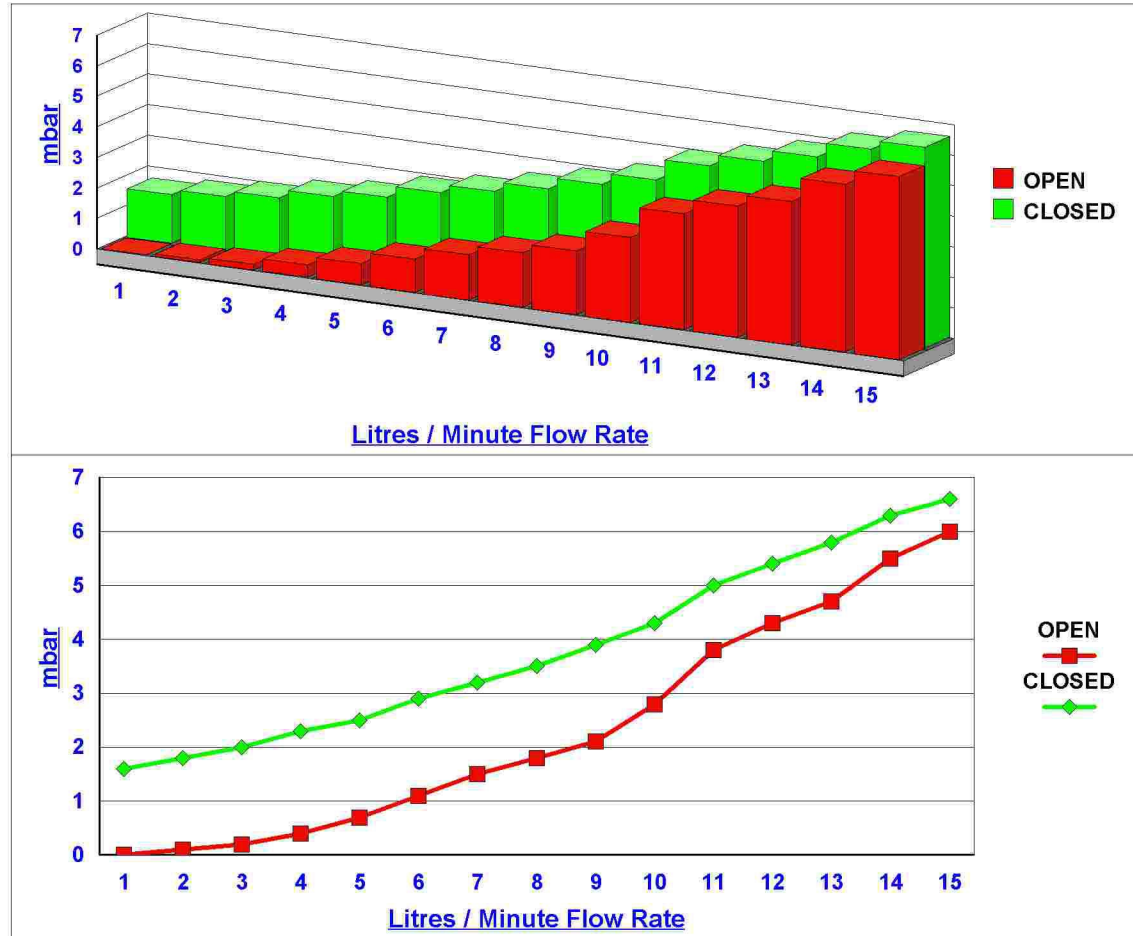

Results of Testing done on Tom Thumb "PEEP" Facility

Readings taken with Valve Fully Closed, and Fully Open (45CmH<sub>2</sub>O)