## NOTES: UNLESS OTHERWISE SPECIFIED.

- 1. LABEL PER CUSTOMER SPECIFICATION
- 2. CONNECTORS POLARITY:
  TIP (CENTER)— NEGATIVE (-)
  SLEEVE POSITIVE (+)


TYPICAL MATING PLUG SWITCHCRAFT .141" MINIATURE PHONE PLUGS P/N: 740 (SCREW TERMINAL) OR P/N: 750 (CLAMP-LUG TERMINAL).


- 3. TEMPERATURE COMPENSATION ERROR IS ±5% OF FULL SCALE OVER THE OPERATING TEMPERATURE RANGE. WORST CASE TRACKING ERROR (WITHIN THE FIRST HOUR AFTER A MAXIMUM TEMPERATURE STEP) IS ±10% OF FULL SCALE. (GAS SAMPLES MUST BE BROUGHT TO AMBIENT TEMPERATURE) PERCENT READOUT IS ONLY WITHIN ±1% AT CONSTANT PRESSURE (E.G. A 10% INCREASE IN PRESSURE WILL RESULT IN A 10% INCREASE IN READING).
- 4. ASSEMBLY TO BE PACKAGED IN A GAS BARRIER BAG.
- 5. ASSEMBLY MANUFACTURED AND TESTED TO MPD-61679.

## SPECIFICATIONS:

- 1) OUTPUT (7-13MV) IN AIR AT 25 °C, SEA LEVEL
- 2) RANGE 0-100% OXYGEN.
- 3) ACCURACY WITHIN +/-1% OF FULL SCALE AT CONSTANT TEMPERATURE AND PRESSURE.
- 4) RESPONSE TIME LESS THAN 6 SECONDS FOR 90% OF FINAL VALUE.
- 5) OFFSET LESS THAN 0.5% OF OXYGEN EQUIVALENT AT 25 °C (77 °F) IN ZERO GAS AFTER 36 SECONDS.
- 6) CROSS INTERFERENCE LESS THAN 1.25% O2 RESPONSE TO: 6% HALOTHANE, 6% ISOFLURANE, 6% ENFLURANE, 7% SEVOFLURANE, 20% DESFLURANE IN 30% O2/70% N20 MIXTURE.
- 7) HUMIDITY 0 TO 99% R.H. (NON-CONDENSING).
- 8) OPERATING TEMPERATURE RANGE 0 TO 40 °C (32 TO 104 °F)
- 9) STORAGE TEMPERATURE 0 TO 50 °C (32 TO 122 °F)
- 10) AVG. EXPECTED CELL LIFE 36 MONTHS IN AIR AT 25 °C AND 50% R.H.
- 11) WEIGHT 1.1 OZ (31 GRAMS)
- 12) LOAD 10K REQUIRED

## Re-Labelled R17 VAN For use in Diving



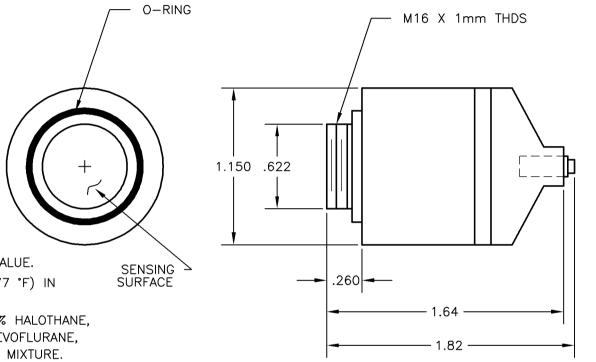

ITEM QTY

PART No.

	BILL OF MATERIAL						
	DO NOT SCALE DWG		THIS DRAWING IS THE PROPERTY OF TELEDYNE ANALYTICAL INSTRUMENTS AND CONTAINS CONFIDENTIAL INFORMATION. IT IS NOT TO BE COPIED, REPRODUCED OR USED WITHOUT WRITTEN PERMISSION.				
	TOLERANCE UNLESS OTHERWISE SPECIFIED: ANGULAR ±1/2*		<b>₹</b> Teledyne Analytical Instruments				
0% R.H.	LINEAR $ \begin{cases} .X = \pm .1 \\ .XX = \pm .02 \\ .XXX = \pm .010 \end{cases} $		A business unit of Teledyne Electronic Technologies				
	$(.XXX = \pm .010)$		CITY OF INDUSTRY, CALIFORNIA 91748				
S/	SIGNATURES	DATE	TITLE			SCALE	NTS
N/	DRFT: LIXA GARCES	4/28/93	SPEC. CONTROL DWG.		NIS		
<b>V</b>	CHK:		]	OXYGEN SENSOR		SIM	
P/	APPR: J.M. LAUER	4/3/95	CLASS R17MED		SHEET 1 OF 1		
0/	ENGR: JAY M. LAUER						
F/	S.O.:		MATL		- · · - · · - ·     · · <del>-</del> ·		REV
REFERENCE	CAD I.D. B4539810				B-45398		$\square$

DESCRIPTION