

NORM
O
REV


— OUTPUT +

SWITCH TO "0" WHEN
NOT IN USE.

RANGE

100mV 10mV
V IV 100mA I
OFF 10mA

OUTPUT ADJUST

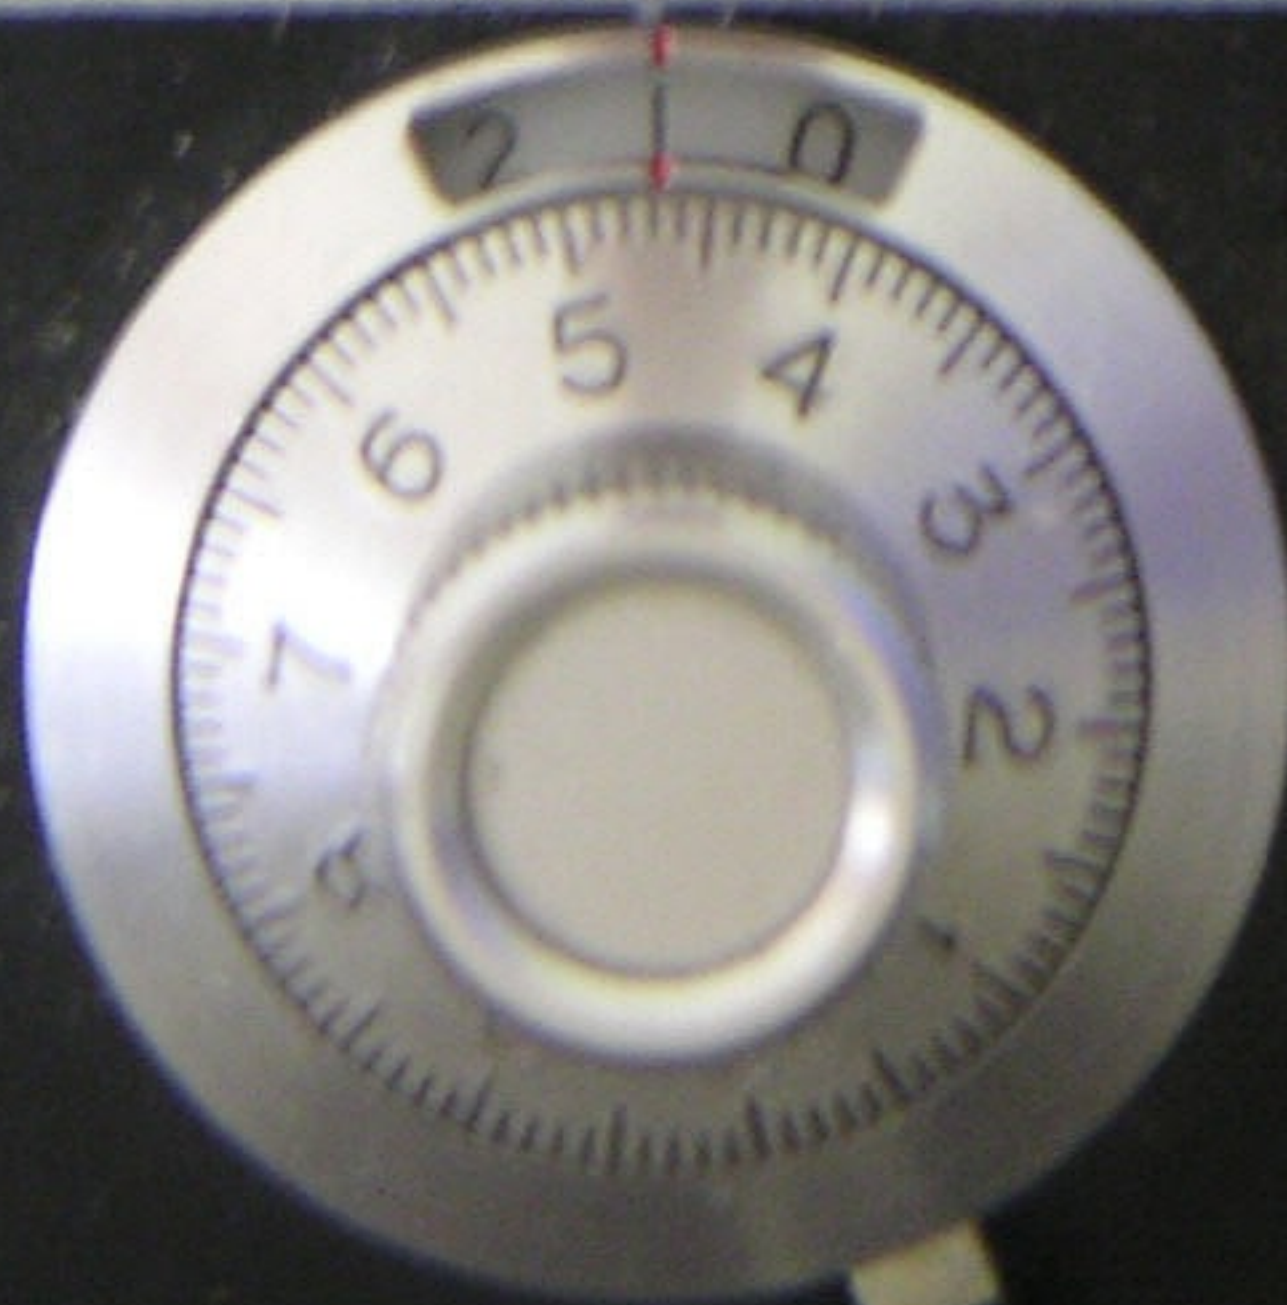

BATT