




**Microstim DB3**  
Supramaximal Nerve Stimulator

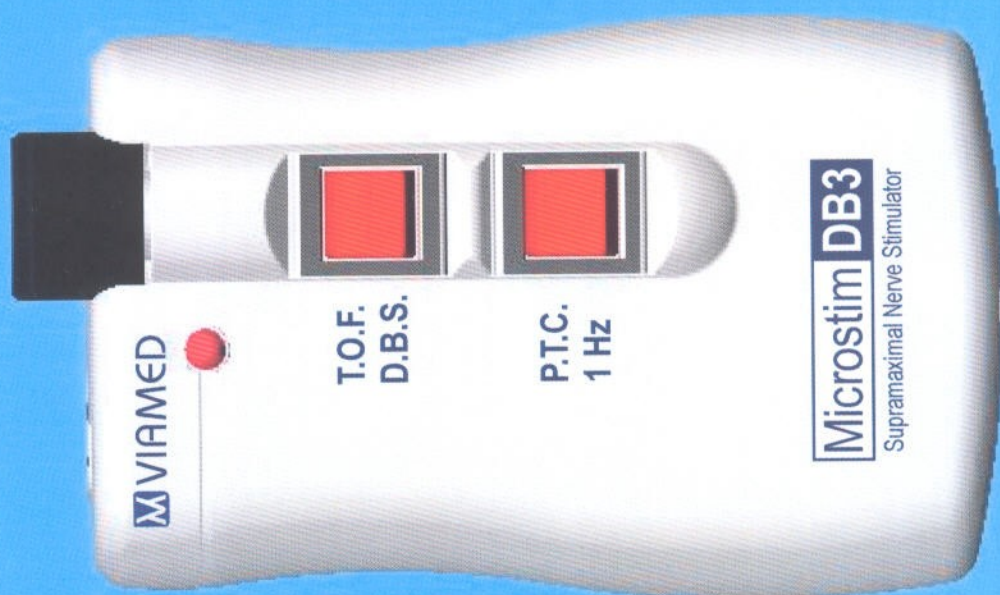


ATTENTION, SEE INSTRUCTIONS FOR USE


Caution when used with cardiac pacemakers.  
Replace battery when indicator flashes red.

CE0086

Viamed, 15 Station Road, Cross Hills, Keighley,  
West Yorkshire, BD20 7DT United Kingdom  
Tel: +44 (0)1535 634642 - Fax: +44 (0)1535 635582  
email: info@viamed.co.uk - web: www.viamed.co.uk

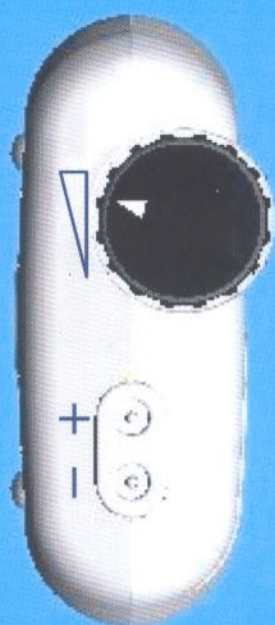



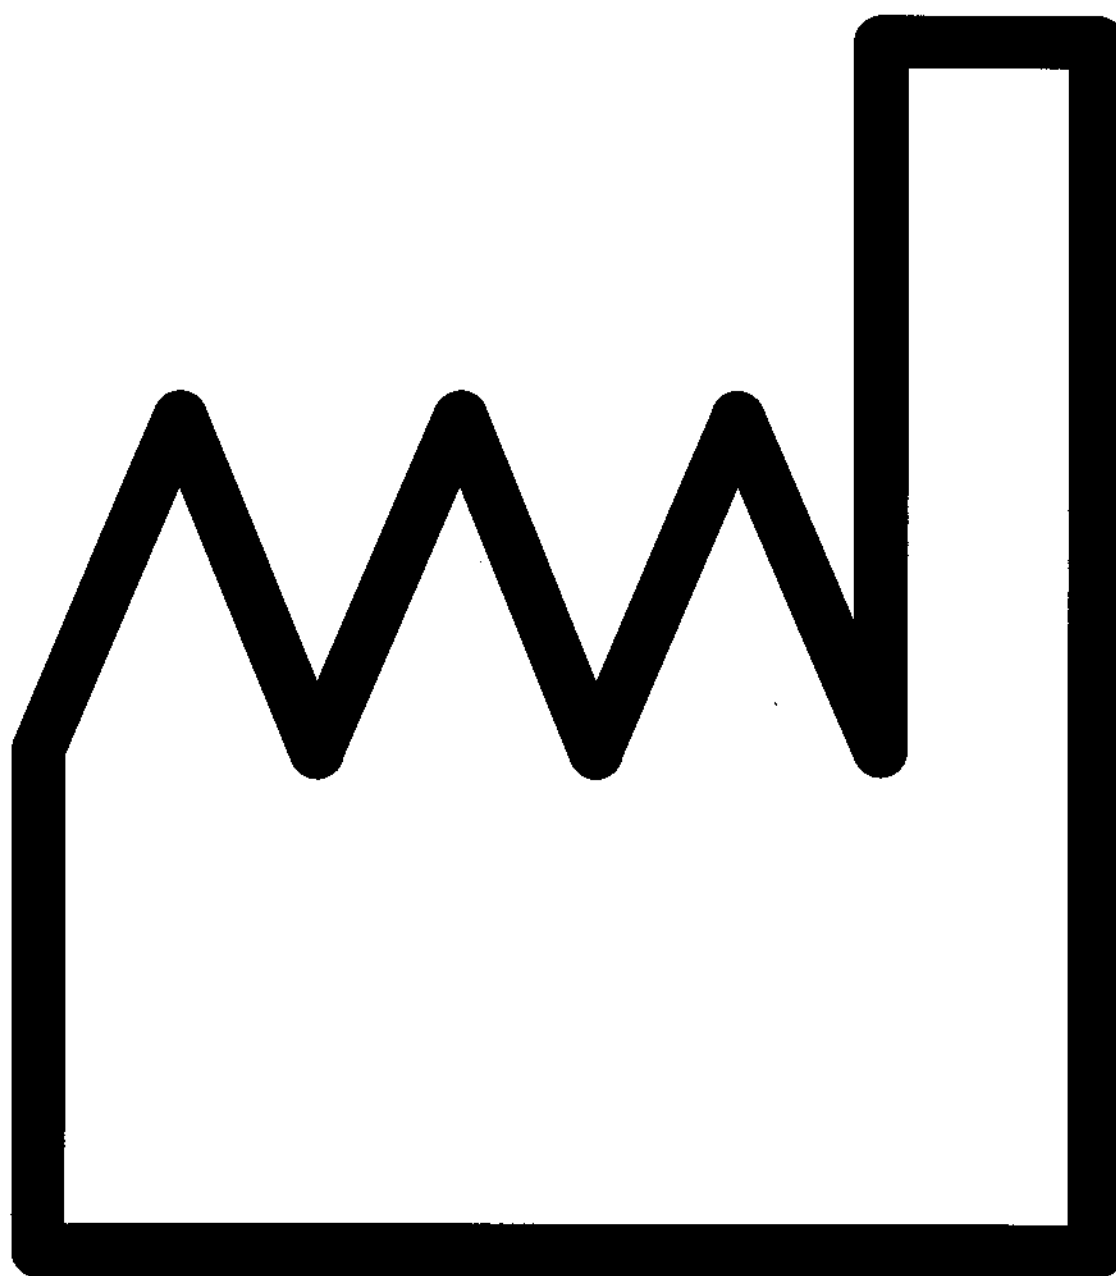





—

+

# **Microstim DB3**

**Supramaximal Nerve Stimulator**



**ATTENTION, SEE INSTRUCTIONS FOR USE**

**Caution when used with cardiac pacemakers.  
Replace battery when indicator flashes red.**


**CE0086**

---

Viamed, 15 Station Road, Cross Hills, Keighley,  
West Yorkshire, BD20 7DT United Kingdom  
Tel: +44 (0)1535 634542 - Fax: +44 (0)1535 635582  
email: [info@viamed.co.uk](mailto:info@viamed.co.uk) - web: [www.viamed.co.uk](http://www.viamed.co.uk)

# Microstim DB3

Supramaximal Nerve Stimulator

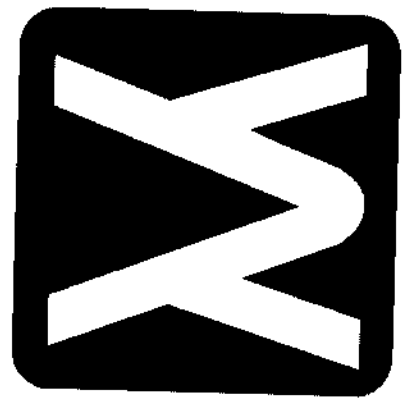 **XBOX** **VIEWED**