


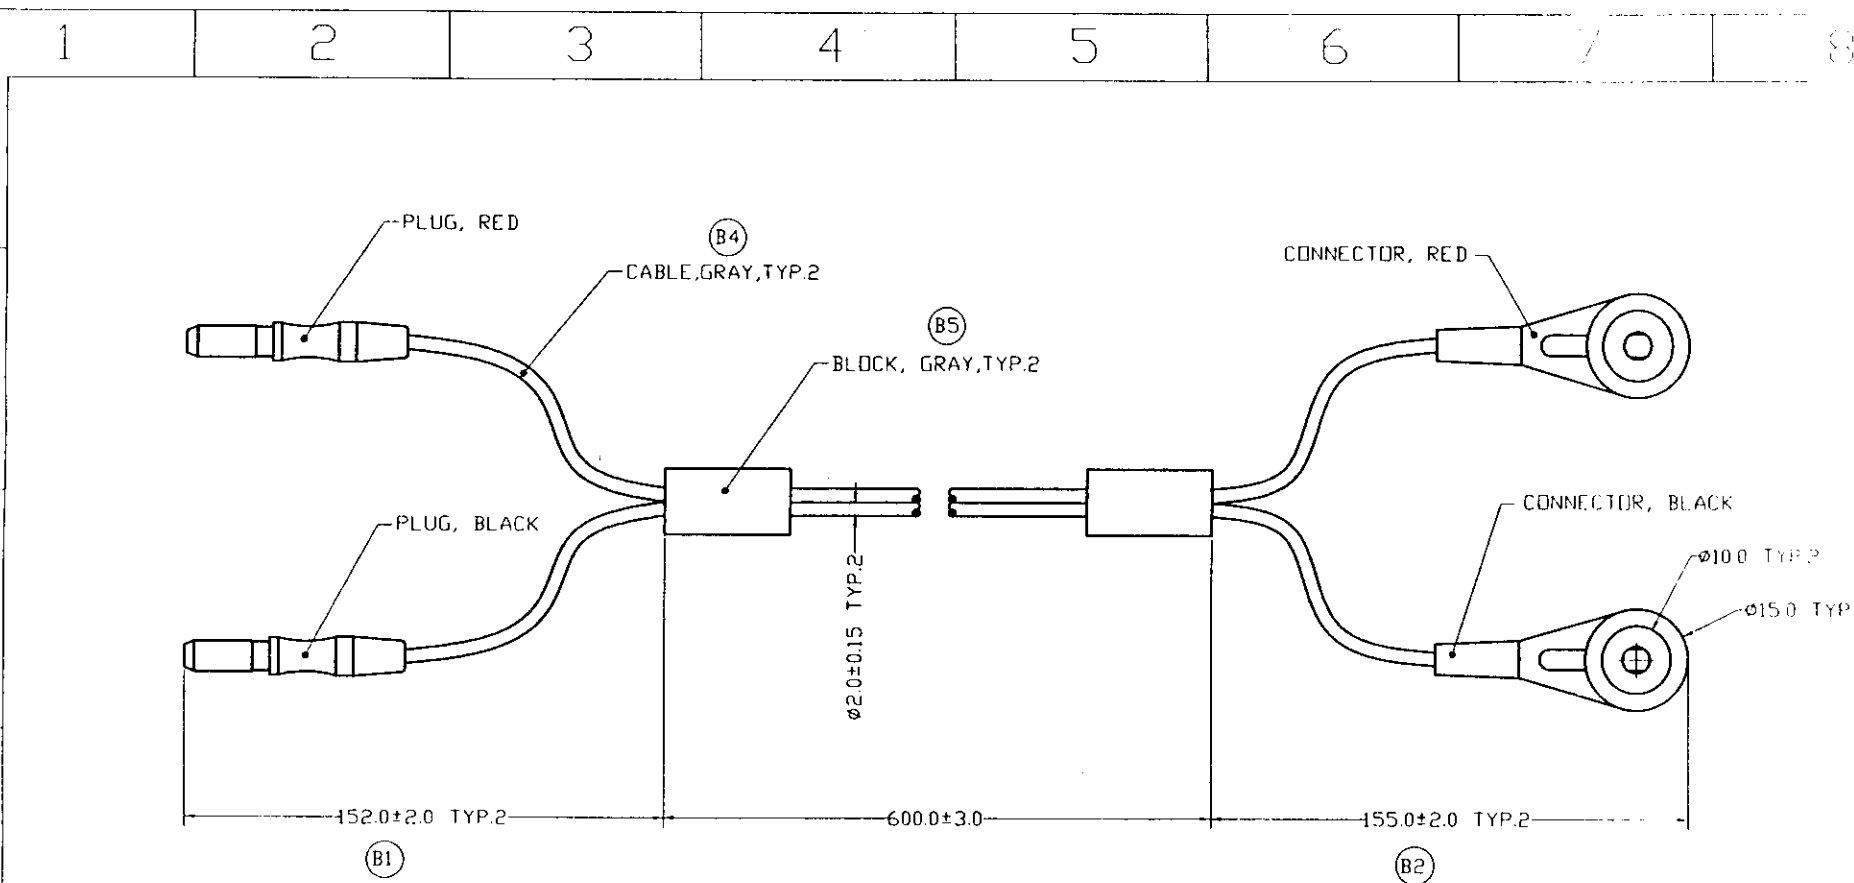

NOTES:

- (1) CABLE MATERIAL: PU
- (2) PLUG: ECG PLUG, NONTTOXIC PVC 90±5 SHORE A.
- (3) BLOCK MATERIAL: PU 60±5 SHORE A.
- (4) HOUSING OF CONNECTOR MATERIAL: PVC 90±5 SHORE A.
- (5) CONNECTOR/ SNAPPER: STAINLESS STEEL.

REV.	85	Gray was white.	Shine Sun	Sep2,05
	84	Gray was white	Shine Sun	Sep2,05
	83	PU was PVC	Shine Sun	Sep2,05
	82	155.0±2.0 WAS 70.00	Shine Sun	Sep2,05
	81	152.0±2.0 WAS 70.00	Shine Sun	Sep2,05
	B	NEW RELEASE		
	A			
		ZONES - CHANGES	ER#	DATE CR

MAT'L		SEE NOTES		UNLESS OTHERWISE STATED		HEALTHCARE TECHNOLOGY INTERNATIONAL L.			
COLOR		TEXTURE		WALL THICKNESS	MM	TITLE	ECG CABLE		
SEE DRAWING				LINEAR	.X	± .02 MM	PROJECT	688	SCALE
HARDNESS		COATING		ANGULAR	XX	± .01 MM	DSGN	7/16/05	SHEET 1 OF 1
PROCESS/JOINING		ROUGHNESS		DRAFT ANGLE / SIDE	1" MAX		CHKR	7/16/05	PART NO
STANDARDS				BURR & FLASH	0.1 MAX		APPD	7/16/05	4C-68660
				BREAK & CORNER	R0.2 MAX				
				PARTING LINE MISMATCH	0.05MAX				