


NOTES: UNLESS OTHERWISE SPECIFIED.

1. LABEL PER CUSTOMER SPECIFICATION
2. CONNECTIONS POLARITY :
TIP (CENTER) - NEGATIVE (-)
SLEEVE - POSITIVE (+)
TYPICAL MATING PLUG SWITCHCRAFT .141" MINIATURE PHONE PLUGS
P/N: 740 (SCREW TERMINAL) OR P/N: 750 (CLAMP-LUG TERMINAL).
3. TEMPERATURE COMPENSATION ERROR IS $\pm 5\%$ OF FULL SCALE OVER THE OPERATING TEMPERATURE RANGE. WORST CASE TRACKING ERROR (WITHIN THE FIRST HOUR AFTER A MAXIMUM TEMPERATURE STEP) IS $\pm 10\%$ OF FULL SCALE. (GAS SAMPLES MUST BE BROUGHT TO AMBIENT TEMPERATURE) PERCENT READOUT IS ONLY WITHIN $\pm 1\%$ AT CONSTANT PRESSURE (E.G. A 10% INCREASE IN PRESSURE WILL RESULT IN A 10% INCREASE IN FULL SCALE).
4. ASSEMBLY TO BE PACKAGED IN A GAS BARRIER BAG.
5. ASSEMBLY MANUFACTURED AND TESTED TO MPD61679.

SPECIFICATIONS:

1. OUTPUT - (7-13MV) IN AIR 25°C AT SEA LEVEL.
2. RANGE - 0-100% OXYGEN (MAX), 0-1% OXYGEN (MIN).
3. RESPONSE TIME - LESS THAN 6 SEC. FOR 90% OF FINAL VALUE.
4. OPERATING TEMPERATURE RANGE - 0° TO 40°C (32° TO 104°F)
5. AVG EXPECTED CELL LIFE - 36 MONTHS IN AIR AT 25°C, 50% R.H.
6. STORAGE TEMPERATURE - 0° TO 50°C (32° TO 122°F)
7. HUMIDITY - 0 TO 99% RH (NON-CONDENSING).
8. ACCURACY - WITHIN $\pm 1\%$ OF FULL SCALE AT CONSTANT TEMPERATURE AND PRESSURE (SEE NOTE 3)
9. WEIGHT - 1.2 OZ (32 GM)
10. OFFSET - $\leq 0.1\%$ O₂ IN ≤ 30 SECONDS FOR A STEP CHANGE FROM AIR TO 0% O₂.
11. REQUIRED LOAD 10K

REVISIONS				
REV	DESCRIPTION	DATE	APP.	REV BY
6	ECO# 94-503	09/01/94	JML	--
7	ECO# 96-0713	6-11-97	M.G.	JCR

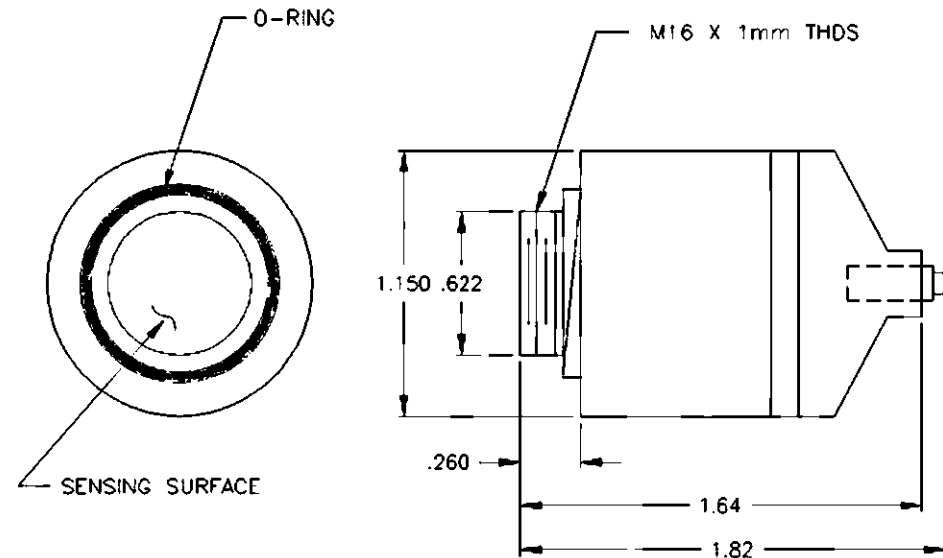

DO NOT SCALE DWG		THIS DRAWING IS THE PROPERTY OF TELEDYNE ANALYTICAL INSTRUMENTS AND CONTAINS CONFIDENTIAL INFORMATION. IT IS NOT TO BE COPIED, REPRODUCED OR USED WITHOUT WRITTEN PERMISSION.																					
TOLERANCE UNLESS OTHERWISE SPECIFIED: ANGULAR $\pm 1/2^\circ$		Teledyne Analytical Instruments A business unit of Teledyne Electronic Technologies CITY OF INDUSTRY, CALIFORNIA 91748																					
LINEAR $\begin{matrix} \text{X} & = & \pm .1 \\ \text{XX} & = & \pm .02 \\ \text{XXX} & = & \pm .010 \end{matrix}$																							
<table border="1"> <tr> <th>SIGNATURES</th> <th>DATE</th> </tr> <tr> <td>DRT: L. GARCES</td> <td>04/28/93</td> </tr> <tr> <td>CHK:</td> <td></td> </tr> <tr> <td>APPR:</td> <td></td> </tr> <tr> <td>ENGR: JAY LAUER</td> <td></td> </tr> <tr> <td>S.O.:</td> <td></td> </tr> <tr> <td>REFERENCE</td> <td>CAD I.D. B56356-7</td> </tr> </table>				SIGNATURES	DATE	DRT: L. GARCES	04/28/93	CHK:		APPR:		ENGR: JAY LAUER		S.O.:		REFERENCE	CAD I.D. B56356-7						
SIGNATURES	DATE																						
DRT: L. GARCES	04/28/93																						
CHK:																							
APPR:																							
ENGR: JAY LAUER																							
S.O.:																							
REFERENCE	CAD I.D. B56356-7																						
<table border="1"> <tr> <td colspan="2">TITLE</td> <td>SCALE</td> </tr> <tr> <td colspan="2">SPEC CONTROL DWG</td> <td>NONE</td> </tr> <tr> <td colspan="2">OXYGEN SENSOR</td> <td>SIM NONE</td> </tr> <tr> <td colspan="2">CLASS R17A</td> <td>SHEET 1 OF 1</td> </tr> </table>		TITLE		SCALE	SPEC CONTROL DWG		NONE	OXYGEN SENSOR		SIM NONE	CLASS R17A		SHEET 1 OF 1	<table border="1"> <tr> <td>MAIL</td> <td>NOTED</td> <td>DWG NO</td> <td>REV</td> </tr> <tr> <td></td> <td></td> <td>B-56356</td> <td>7</td> </tr> </table>		MAIL	NOTED	DWG NO	REV			B-56356	7
TITLE		SCALE																					
SPEC CONTROL DWG		NONE																					
OXYGEN SENSOR		SIM NONE																					
CLASS R17A		SHEET 1 OF 1																					
MAIL	NOTED	DWG NO	REV																				
		B-56356	7																				