



Old

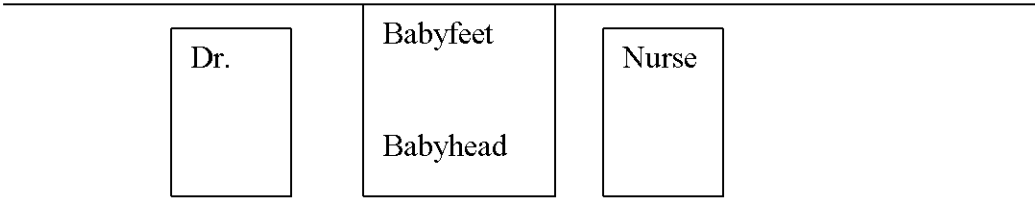

ew

N

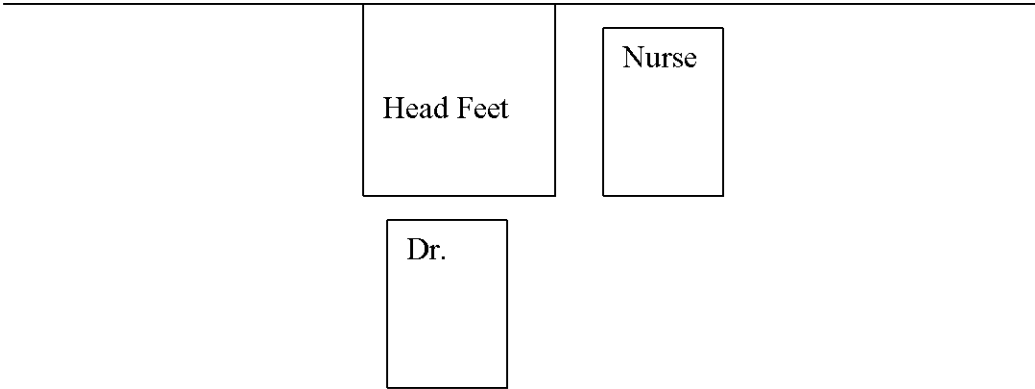

Two requests for changing the Viamed resuscitation cabinet.

The first request:

Since 2007 the method of resuscitation (ALS-neonatal) has changed.

We used to do neonatal hart massage with two fingers standing on side along to the body of the baby.(see schedule: Old)

Now we have to do hart massage standing at the feet of the baby holding the chest to do hart massage.(see schedule: New)

For that reason we would like to have a rotatable table in the cabinet.

The second request is:

The plastic holders round the mattress should have the same height as the mattress itself.

The reason for this request is the following:

The high plastic holders hinder our work with the baby. Without them we have a better work floor.

The cabinet is only used for resuscitation. The baby will never be left alone on the cabinet.

Yours sincerely,

Siemen Goosensen
Staff Nurse Obstetrics
Ziekenhuis Zeeuws Vlaanderen
Terneuzen
siemen@zzv.nl