


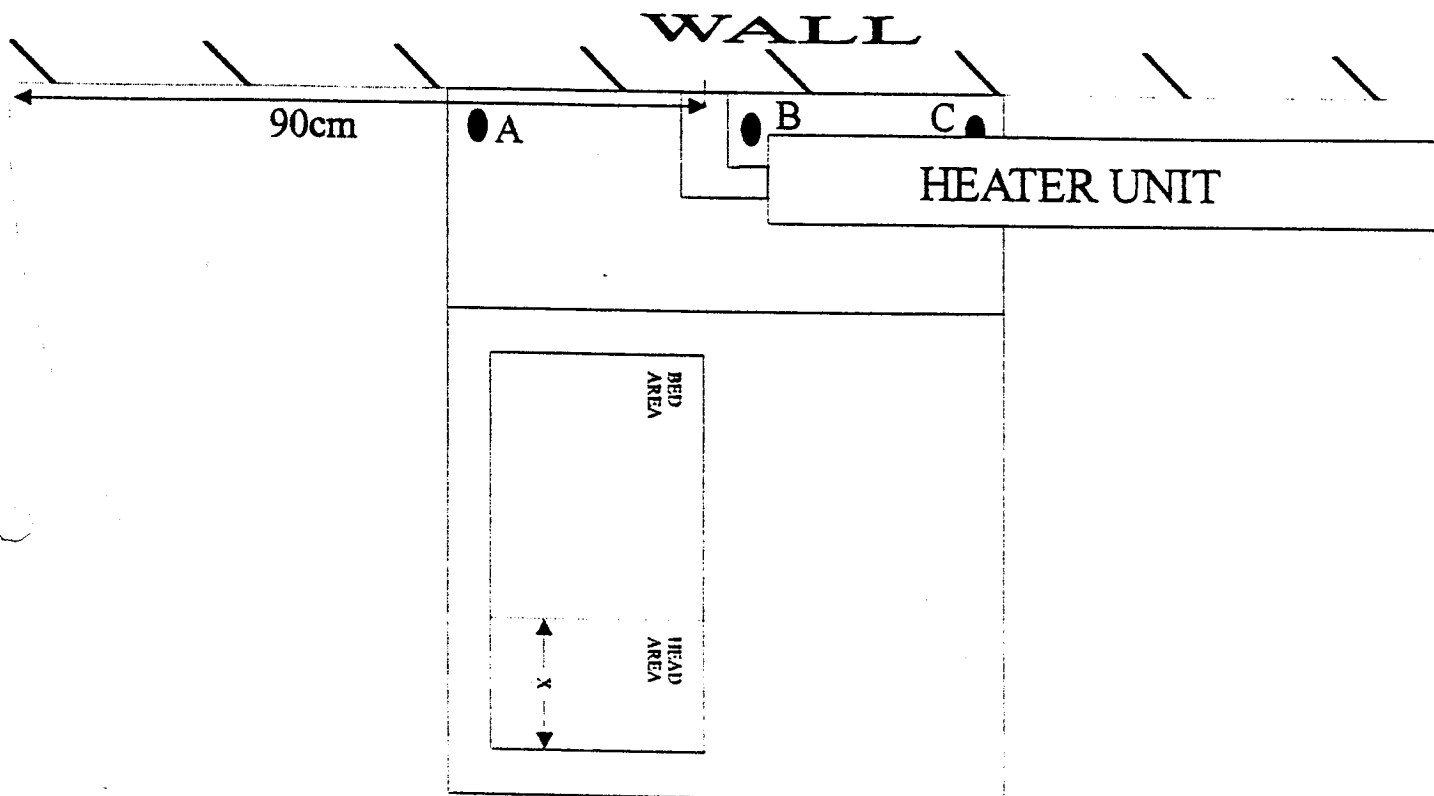

Position of insert Holes
For Oxygen and Suction Hoses

A


Yes / No

B

Yes / No

C

Yes / No

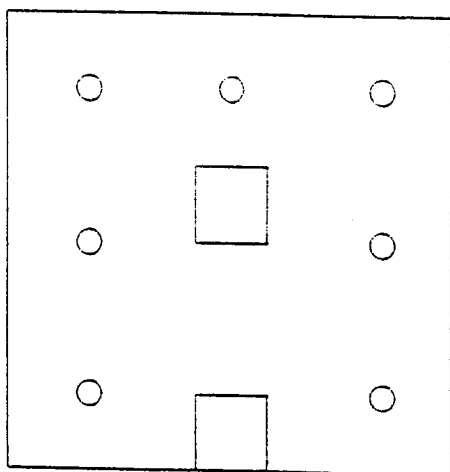

Wall plate for heater
Can be mounted in position shown
i.e. 84cm above the bed
or turned 180° 72cm above the bed

Contact	
Date	12.7.95
Hospital	
Engineer	
Diagram	TC004