


MICROSTIM DB3 TESTER SCHEMATIC V2.0

HLNP-ED27-TW000

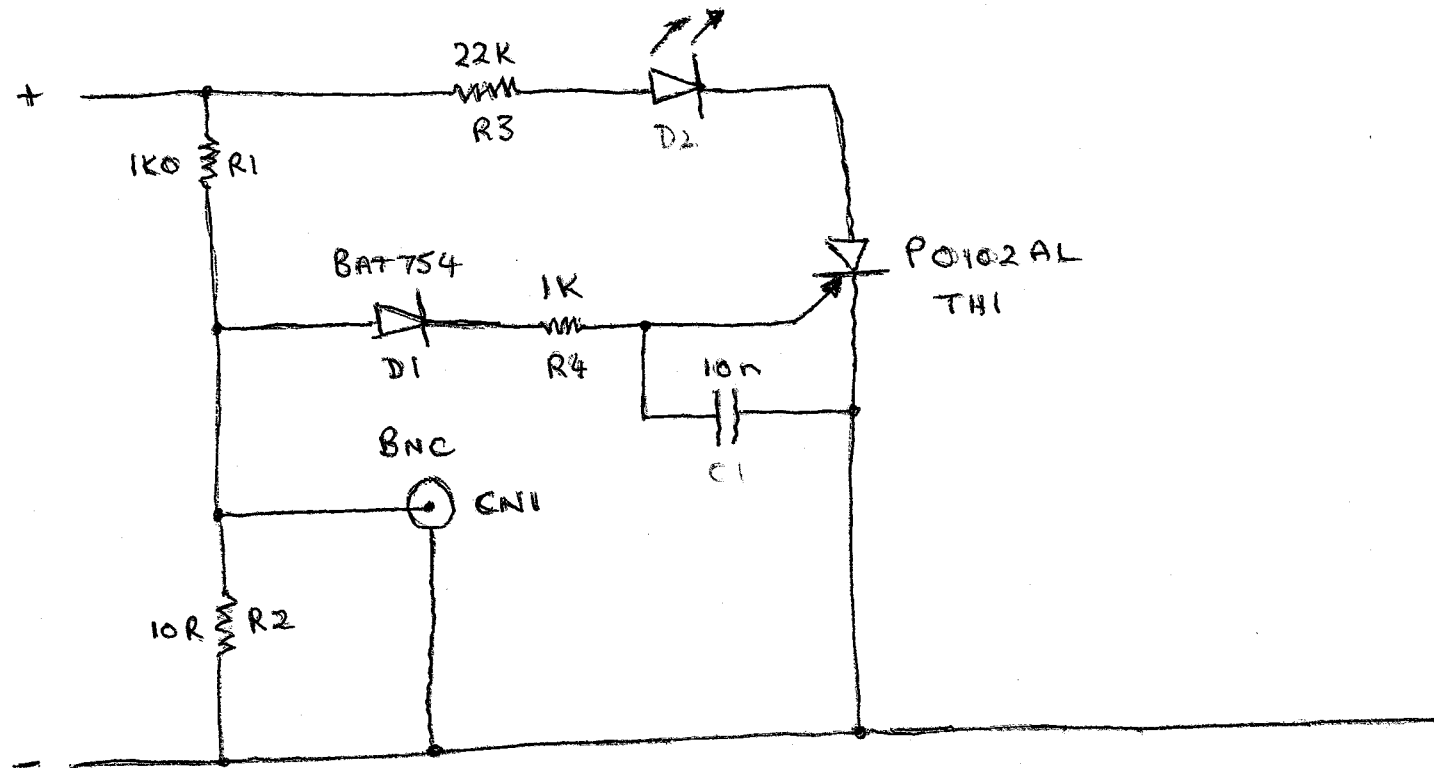

REV: 1.0

P. ANDERSON

3rd JULY 2007

REV 2.0

P. ANDERSON

5th September 2007

R3 CHANGED FROM 1K8 TO 22K R4 $\Rightarrow$ 1K Ω FROM 100 Ω C1 ADDED