

Viamed VM-2500-S Series Capnograph

Serial number: **80940146**
 Firmware: **v8.8**

RMA: **2020-0258**
 Document No.: **33998**
 Number: **2021-20015**

Gas Accuracy Check


Service number: **4480520**

Test	Range	Displayed value EtCO ₂ /FiCO ₂	Result
Calibration gas 5% +/- 0.1vol% CO ₂ , 20.9% O ₂ , balance N ₂	EtCO ₂ : 4.7 - 5.3 vol% FiCO ₂ : 0.0 - 0.3vol%	4.7 % / 0.2 %	PASS
Breaths per minute	10 (+/- 1bpm)	10	PASS
ISA module leakage test	CO ₂ drop <0.5vol% over 1 minute		PASS

Visual inspection	PASS
Power supply checks	PASS
SpO ₂ functionality	PASS
Alarms and data download functionality	PASS

Certificate number: **1611844410**

Signed:

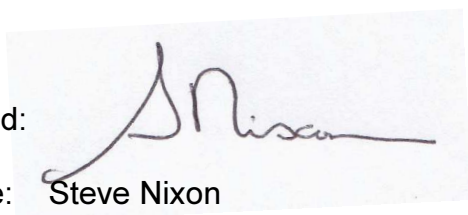

Name: Steve Nixon

Position: Director

Date: 28th January 2021