


Oxygen Sensor Model	PSR-11-75-PO2R
Measuring Range	0-100% O ₂
Signal Output (1)	4-8mV
Response Time 90%	13 seconds
Accuracy Full Scale (2)(4)	± 1%
Accuracy Over Operating Range	± 5%
Drift % Signal/Month (2)(3)	< 1%
Linearity	± 1%
Flow Rate Recommended	0.1–10 lpm
Position Sensitivity (3)	None
Temperature Coefficient	Compensated
Operating Range	0 to 50° C
Pressure	Ambient
Humidity Non-Condensing	0-99% RH
Expected Life (1)	60 months
Storage Temperature (5)	0 to 40°C
Warranty ex-factory (6)	12 months
Electrical Connections	Conn-1007

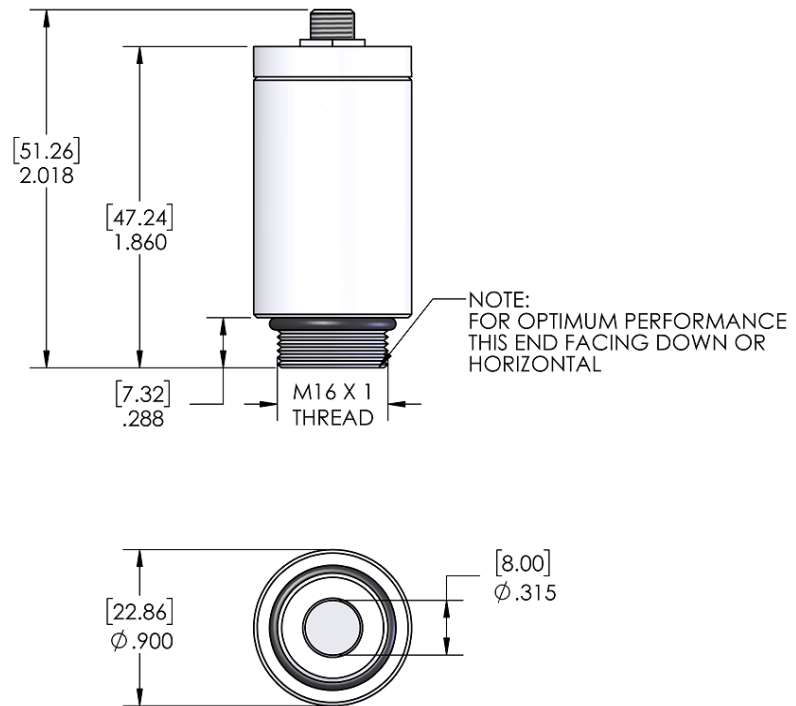

Specifications validated during design and in the pursuit of improvement are subject along with prices to change without notice.

(1) In air (20.9% oxygen) at 25° C and 1 atm.

(2) At constant temperature, pressure and humidity, when calibrated at 100%.

(3) For optimum performance at elevated oxygen levels > 40%, calibrate with 100% oxygen.

(4) From the Signal Output (1) value established above, and, once the sensor reaches equilibrium (approximately 1 hour) following step change of 15°C or more.

(5) Sensors may be stored up to 55°C on an intermittent (up to one week) basis only, such as during transportation. Refer to (1) relative to the Expected Life.

(6) Ex-Factory unless otherwise agreed to in writing. Under normal operating conditions for medical oxygen delivery equipment the sensors are warranted to be free of defects in materials and workmanship for the specified period above provided the sensor is properly installed and operated. The sole remedy for a sensor determined to be defective by Analytical Industries Inc. is limited to replacing the defective sensor. Analytical Industries Inc. shall not be liable for buyer's negligence, misapplication, alteration, abuse or accident.

Rev 201013