


30th May 2019

Viamed Oxygen Sensors Packaging & Sensor Labelling

0110014 R-15V

Medical Oxygen Sensor R- 15V


REF 0110014
SN V123456



(01)04036616000345(11)190301(21)V123456


CE 0123

Tel: +44 (0)1535 634542
 Email: info@viamed.co.uk Website: www.viamed.co.uk

EnviteC-Wismar GmbH
 Alter Holzhafen 18
 D-23966 Wismar
 www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm


Medical Oxygen Sensor R- 15V

REF 0110014
SN: V123456





Tel: +44 (0)1535 634542
 Email: info@viamed.co.uk
 Website: www.viamed.co.uk

EnviteC-Wismar GmbH
 CE 0123

2019-03

Sensor label: 90 x 15 mm




Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110018 R-17V

Medical Oxygen Sensor R- 17V

      2019-03-01

REF 0110018 SN V123456



(01)04036616000383(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 17V

REF 0110018 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110019 R-17Vi

Medical Oxygen Sensor R- 17Vi

      2019-03-01

REF 0110019 SN V123456



(01)04036616000369(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 17Vi

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

REF 0110019 SN: V123456

 EnviteC-Wismar GmbH
CE 0123



   2019-03

Sensor label: 90 x 15 mm




Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110020 R-22Vi

Medical Oxygen Sensor R- 22Vi

REF 0110020 SN V123456 2019-03-01



(01)04036616000352(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 22Vi

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

REF 0110020 SN: V123456

 EnviteC-Wismar GmbH
CE 0123



 2019-03

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110021 R-22MEDV

Medical Oxygen Sensor R- 22MEDV

      2019-03-01

REF 0110021 SN V123456



(01)04036616000376(11)190301(21)V123456

VIAMED CE 0123

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 22MEDV

REF 0110021 SN: V123456



 EnviteC-Wismar GmbH
CE 0123

   2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110023 R-23V

Medical Oxygen Sensor R- 23V

      2019-03-01

REF 0110023 SN V123456



(01)04036616000499(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1636 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 23V

REF 0110023 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03


Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110025 R-23Vi

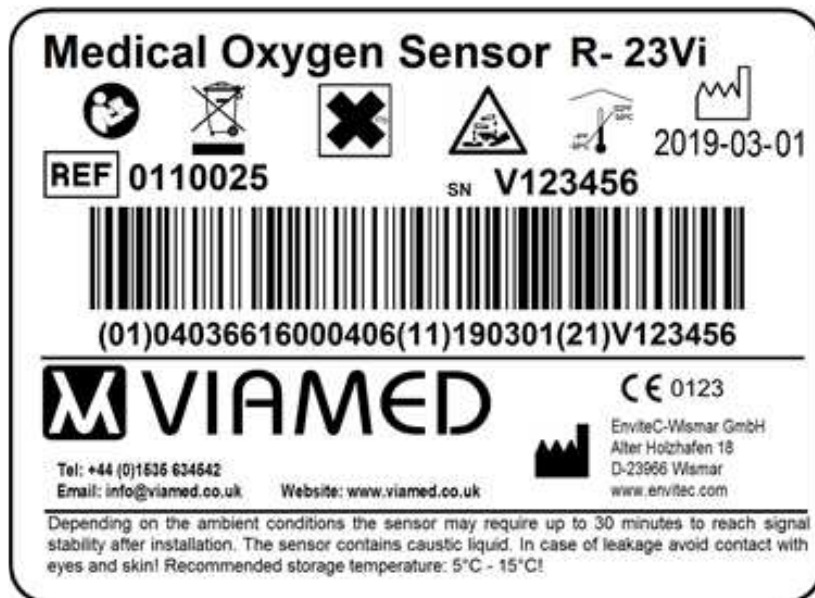

Packaging label: 63.5 x 46.6 mm



Sensor label: 90 x 15 mm

0110039 R-22VA








Medical Oxygen Sensor R- 22VA

REF 0110039 SN V123456 2019-03-01



(01)04036616010740(11)190301(21)V123456


VIAMED

CE 0123

EnviteC-Wismar GmbH
 Alter Holzhafen 18
 D-23966 Wismar
 www.envitec.com

Tel: +44 (0)1535 634542
 Email: info@viamed.co.uk Website: www.viamed.co.uk

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm


VIAMED

Tel: +44 (0)1535 634542
 Email: info@viamed.co.uk
 Website: www.viamed.co.uk

Medical Oxygen Sensor R- 22VA

REF 0110039 SN: V123456

EnviteC-Wismar GmbH
 CE 0123






2019-03

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110040 R-30V

Medical Oxygen Sensor R- 30V

      2019-03-01

REF 0110040 SN V123456



(01)04036616000482(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

 EnviteC-Wismar GmbH

   CE 0123

2019-03

Medical Oxygen Sensor R-30V

REF 0110040

SN:  V123456

Sensor label: 39.8 mm diameter



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110041 R-41V

Medical Oxygen Sensor R- 41V

      2019-03-01

REF 0110041 SN V123456



(01)04036616000512(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 41V

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

REF 0110041 SN: V123456

 EnviteC-Wismar GmbH
CE 0123 

   2019-03

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110042 R-42V

 Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk	Medical Oxygen Sensor R- 42V		  2019-03
	REF 0110042  EnviteC-Wismar GmbH CE 0123	SN: V123456 	

Packaging label: 90 x 15 mm

 Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk	Medical Oxygen Sensor R- 42V		  2019-03
	REF 0110042  EnviteC-Wismar GmbH CE 0123	SN: V123456 	

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110043 R-43V

Medical Oxygen Sensor R- 43V

      2019-03-01

REF 0110043 SN V123456



(01)04036616004596(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 43V

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

REF 0110043 SN: V123456

 EnviteC-Wismar GmbH
CE 0123



   2019-03

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110044 R-44V

Medical Oxygen Sensor R- 44V

REF 0110044 SN V123456 2019-03-01



(01)04036616000529(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 44V

REF 0110044 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110045 R-45V

Medical Oxygen Sensor R- 45V

      2019-03-01

REF 0110045 SN V123456



(01)04036616000420(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1635 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 45V

REF 0110045 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110047 R-47V

Medical Oxygen Sensor R- 47V

      2019-03-01

REF 0110047 SN V123456



(01)04036616000543(11)190301(21)V123456

VIAMED CE 0123

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 47V

REF 0110047 SN: V123456

 EnviteC-Wismar GmbH
CE 0123 

 2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm

0110048 R-48V








Medical Oxygen Sensor R- 48V

REF 0110048 SN V123456 2019-03-01



(01)04036616010122(11)190301(21)V123456



 0123
 EnviteC-Wismar GmbH
 Alter Holzhafen 18
 D-23966 Wismar
 www.envitec.com

Tel: +44 (0)1535 634542
 Email: info@viamed.co.uk Website: www.viamed.co.uk

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

 Tel: +44 (0)1535 634542 Email: info@viamed.co.uk Website: www.viamed.co.uk	Medical Oxygen Sensor R- 48V REF 0110048 SN: V123456  EnviteC-Wismar GmbH  0123	   2019-03
		

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110049 R-49V

Medical Oxygen Sensor R- 49V

      2019-03-01

REF 0110049 SN V123456



(01)04036616000505(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 49V

REF 0110049 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110058 T-7V

Medical Oxygen Sensor T-7V

      2019-03-01

REF 0110058 SN V123456



(01)04036616000413(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor T-7V

REF 0110058 SN: V123456



  2019-03

 EnviteC-Wismar GmbH
CE 0123

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm



Viamed Limited - 15 Station Road - Cross Hills
Keighley -West Yorkshire BD20 7DT - United Kingdom
Tel: +44 1535 634542 Fax: +44 1535 635582
Email: info@viamed.co.uk Website: www.viamed.co.uk

0110075 R-75V

Medical Oxygen Sensor R- 75V

      2019-03-01

REF 0110075 SN V123456



(01)04036616000307(11)190301(21)V123456

VIAMED CE 0123

Tel: +44 (0)1635 634542
Email: info@viamed.co.uk Website: www.viamed.co.uk

 EnviteC-Wismar GmbH
Alter Holzhafen 18
D-23966 Wismar
www.envitec.com

Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!

Packaging label: 63.5 x 46.6 mm

VIAMED Medical Oxygen Sensor R- 75V

REF 0110075 SN: V123456

 EnviteC-Wismar GmbH
CE 0123  2019-03

Tel: +44 (0)1535 634542
Email: info@viamed.co.uk
Website: www.viamed.co.uk

Sensor label: 90 x 15 mm