

Tom Compas

From: Mike A Gonzalez
Sent: Friday, February 12, 2010 12:10 PM
To: Steve Broy
Cc: Tom Compas; Zhenhe Sun
Subject: RE: R22D-AP Testing
Attachments: R22D-AP TComp 2-12-10.xls; B77322-0 R22D-AP Spec.pdf

Steve/Tom,

Testing on three (3) R22D-AP sensors has been completed.


Here is a summary of Results (actual data & chart can be seen on attachment 1:
Note duration time at each temp setting = 3 hours, sensor readings in mV.

Temp, C	Sen #1 Reading	O2 % Error	Sen #2 Reading	O2 % Error	Sen #3 Reading	O2 % Error
Ref 20	10.783	Ref	10.813	Ref	10.370	Ref
0	10.197	-1.1	10.281	-1.0	9.873	-1.0
40	11.089	0.6	11.051	0.5	10.658	0.6

Conclusion:

- All three sensors Sen #1, 2 & 3 gave comp error going from 20 deg C (ref) to cold cycle 0 deg C: **-1.0 to -1.1% O2.**
- All three sensors Sen #1, 2 & 3 gave comp error going from 20 deg C (ref) to hot cycle 40 deg C: **+0.5 to +0.6% O2.**
- As can be seen, test results on 3 R22D-AP look good (see Spec Control dwg attachment 2).

R22D-AP Sensors: Temp Comp test 2-11-10 to 2-12-10,
0-40 deg C, Chart: Time vs mV readings

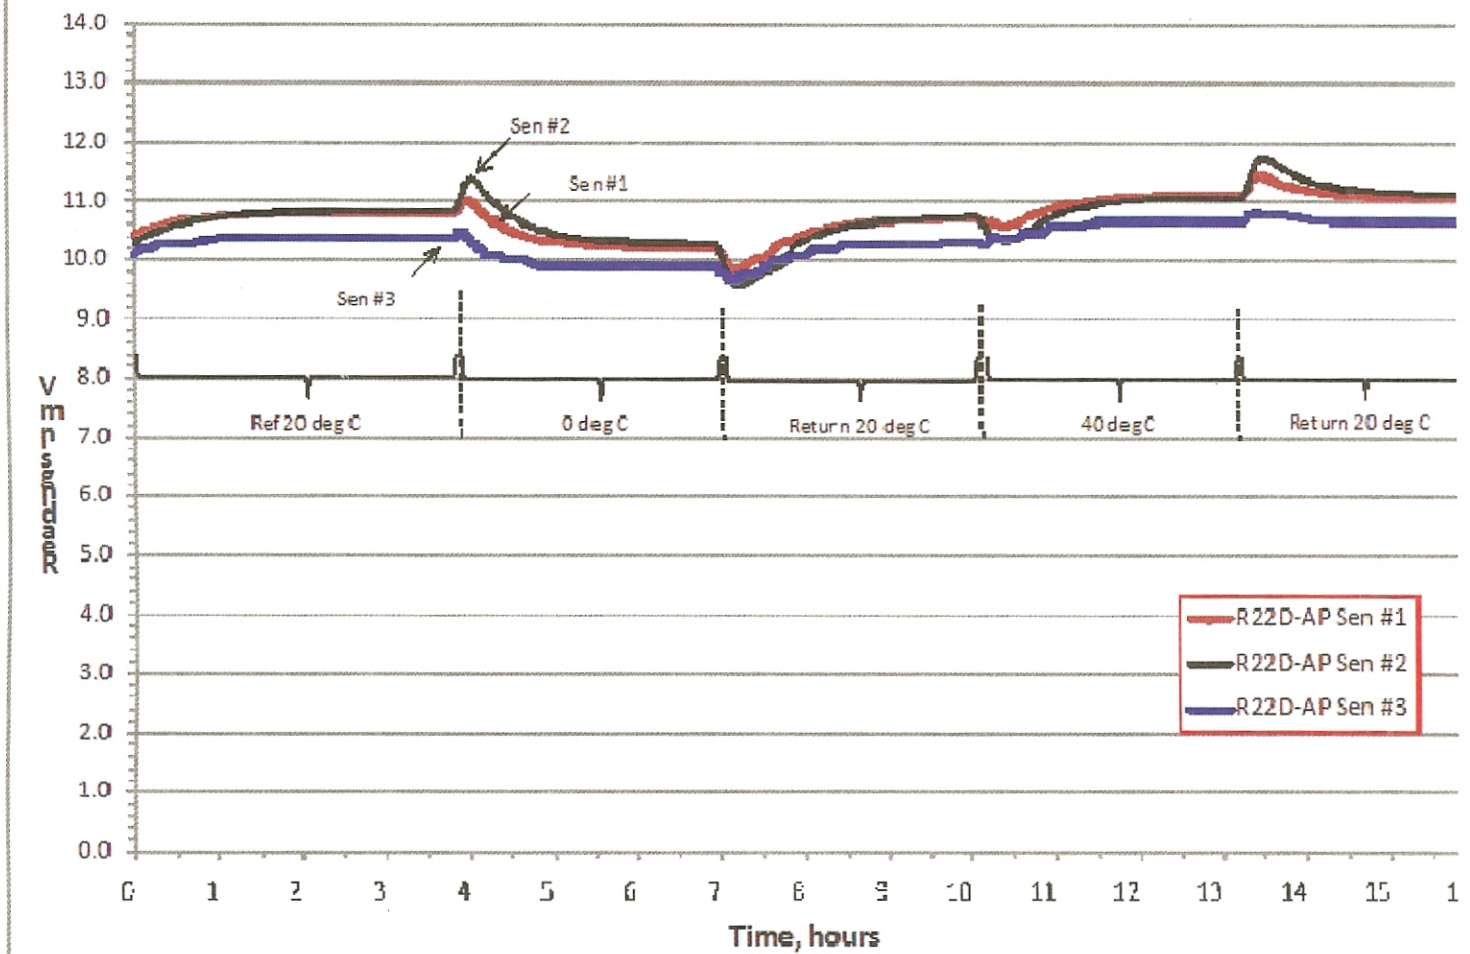

Michael

From: Steve Broy
Sent: Thursday, February 11, 2010 1:32 PM
To: Mike A Gonzalez
Cc: Tom Compas; Zhenhe Sun
Subject: Re: R22D-AP

A diver complained to AP that our cells seems different in temp comp recently
 - although the differences in construction are very minor and hard to imagine this would be contributory, we want to do an A B comparison

From: Mike A Gonzalez
To: Steve Broy
Cc: Tom Compas; Zhenhe Sun
Sent: Thu Feb 11 13:21:27 2010
Subject: RE: R22D-AP
 Steve,

