


Standard TT. #90
15" out on End.

Appr of 285 - 290

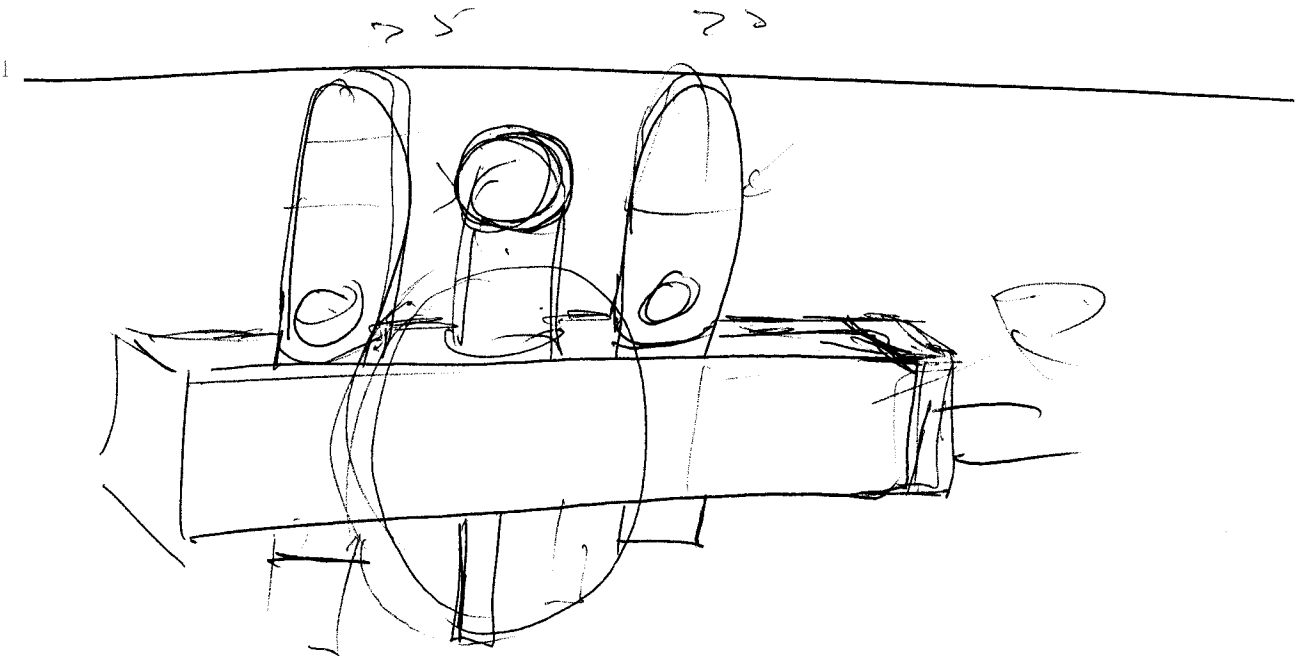

TT Blender

Partly of Flammelin 2

Partly of Blender

Cost TT - 75 app



VIAMED



Drager Tom Thumb Blender Pt.No: DB001

This unit is a simple Air Oxygen Blender

It comprises:-

The main block ,

0-5 ltrs/min Oxygen flowmeter no hose,

0-5 ltrs/min Air flowmeter no hose,

Safety valve


Adjustable valve

15 mm Male outlet. right hand side


Addition holes will be blanked off with blanking plates

Holes in the reverse for mounting Drager Bracket.

BLANKING
PLATE
PT NO 4450-12

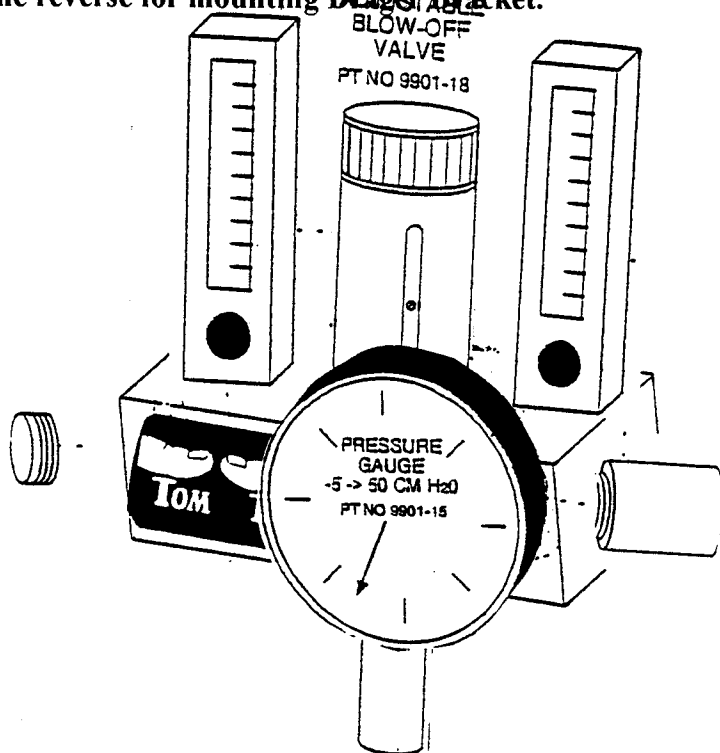


SAFETY
BLOW-OFF
VALVE
PRESET 20 - 30 CM H₂O
PT NO 9901-17

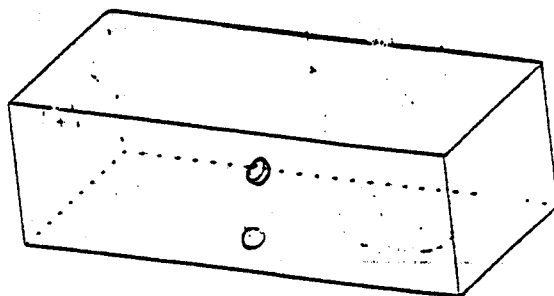


Viamed Limited, 15 Station Road, Cross Hills,
Keighley, West Yorkshire BD20 7DT
Tel: +44 (0) 1535 634542/636757 Fax: +44 (0) 1535 635582
Registration No. 1291765 in England

Trunk 2 125

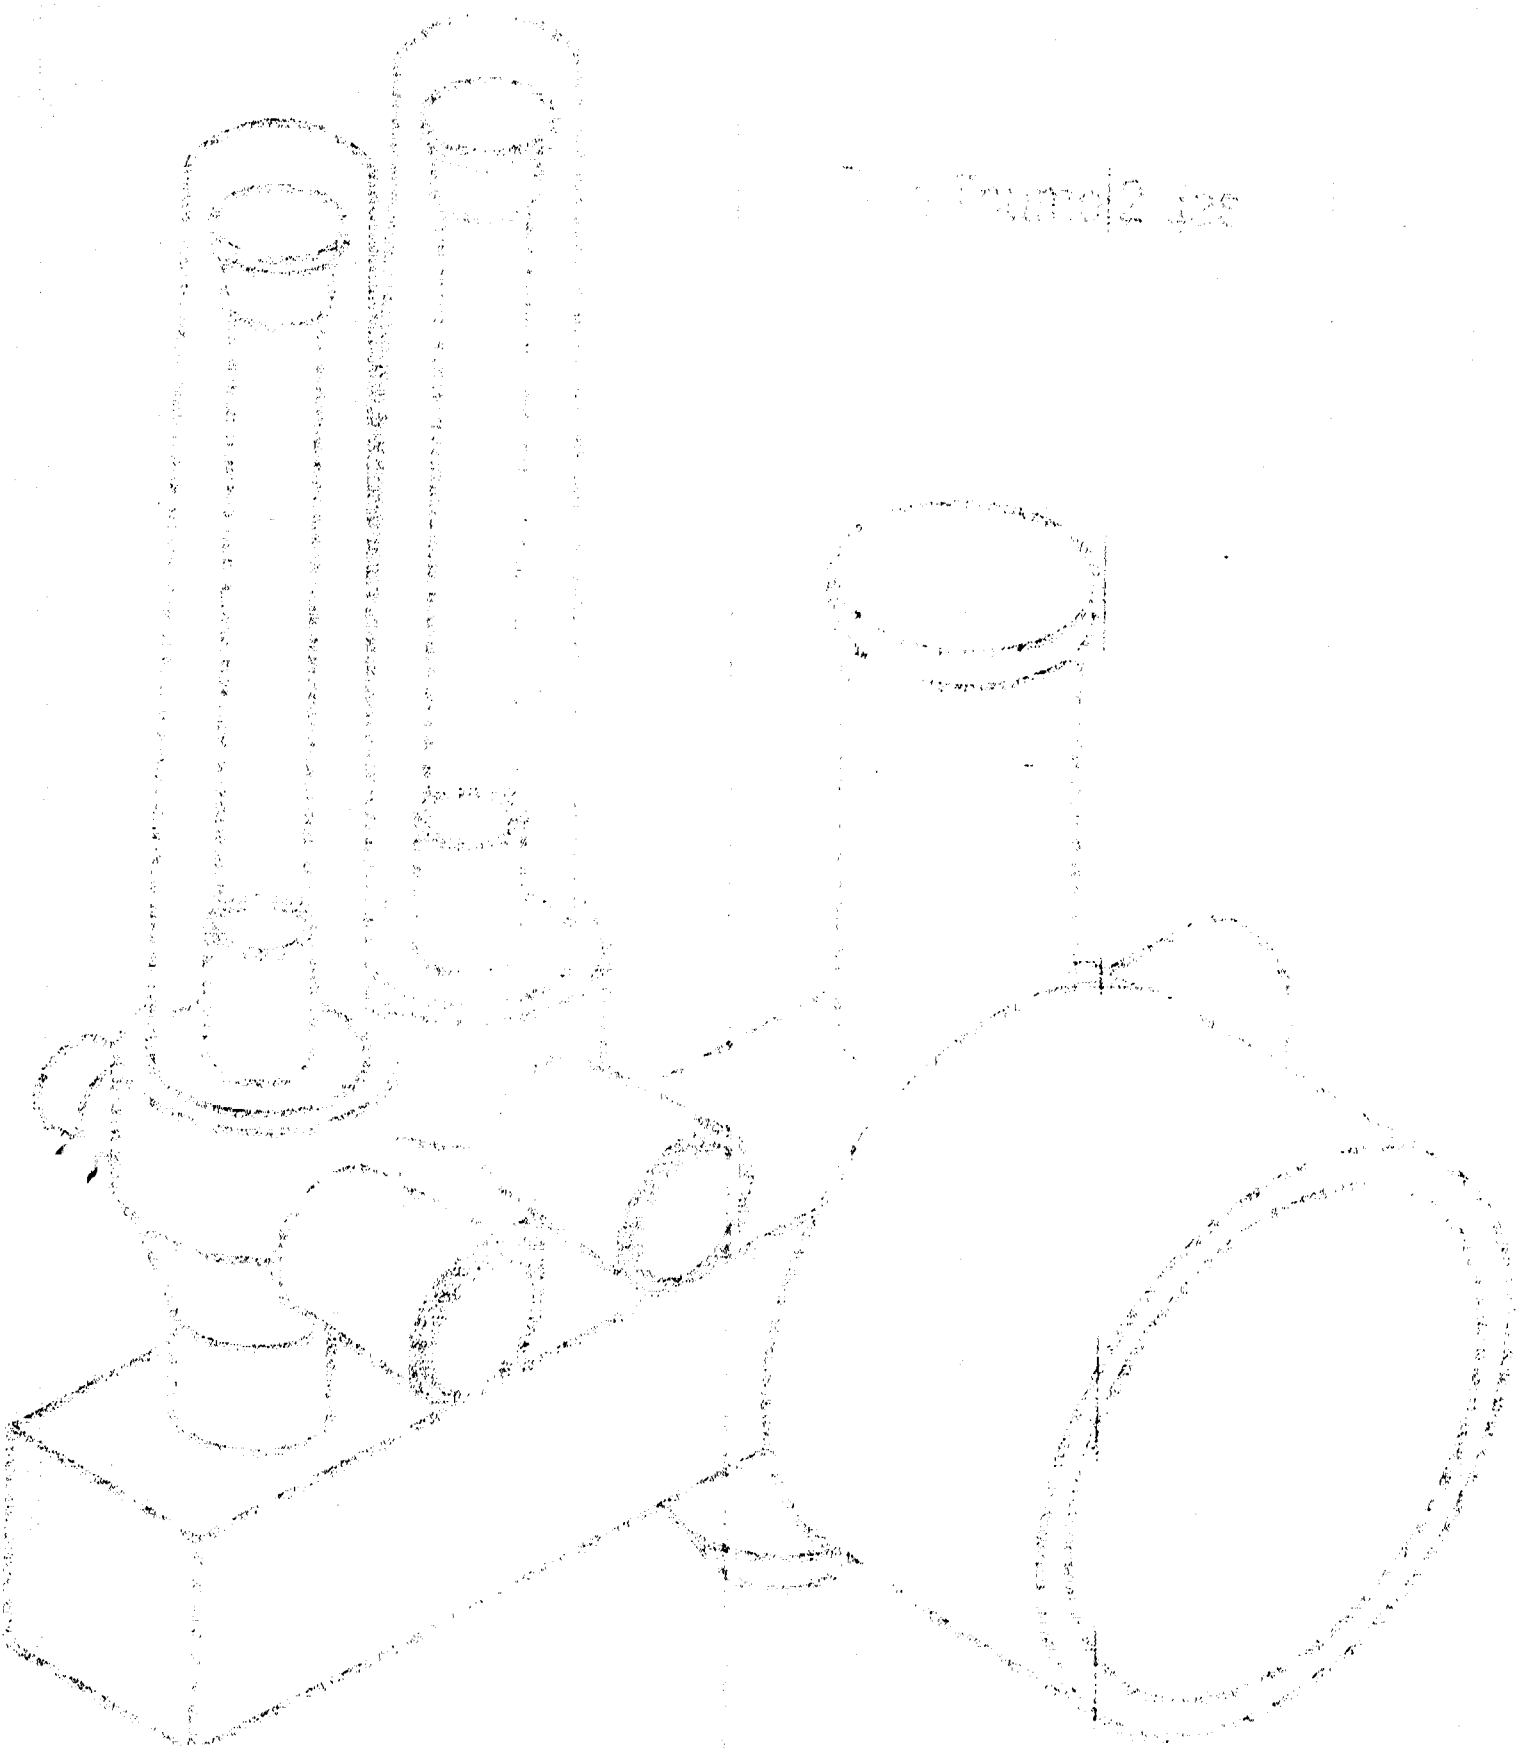


109
off

16mm
A/F

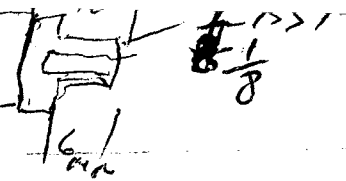


TT495

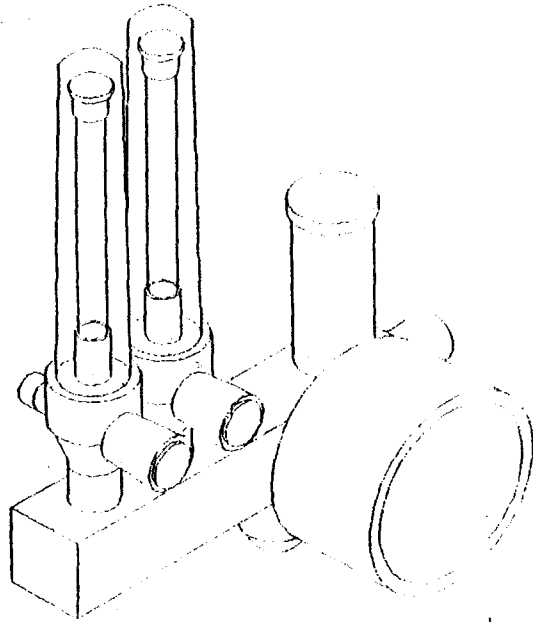

Holes tapped M5 in rear face

Hole
no longer
needed

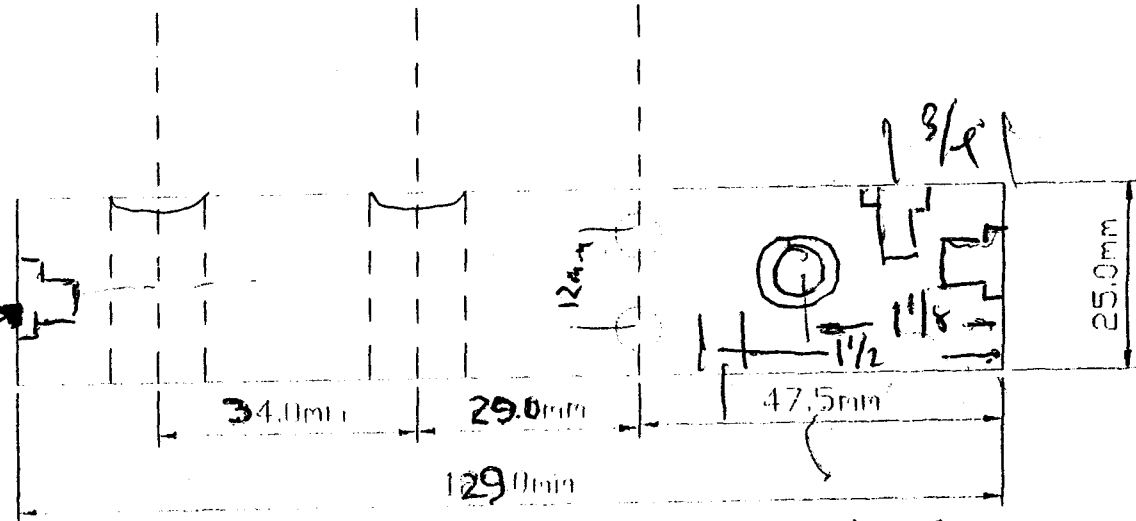

1/8 RSP

SPECIFICATIONS

Position of critical parts.

CONTRACT NO.	DATE	COMPANY Dräger Medical		
DRAWN BY JF		TITLE Ton Thumb Oxygen / Air		
CHECKED BY		SIZE A4	FSCH NO.	DWG NO. / FILE NAME
DESIGNED BY		SCALE 1mm = 1mm	DATE 7/6/97	SHEET 1 of 1
DESIGN ACTIVITY				
CUSTOMER				

TT495