



# Head Boxes.

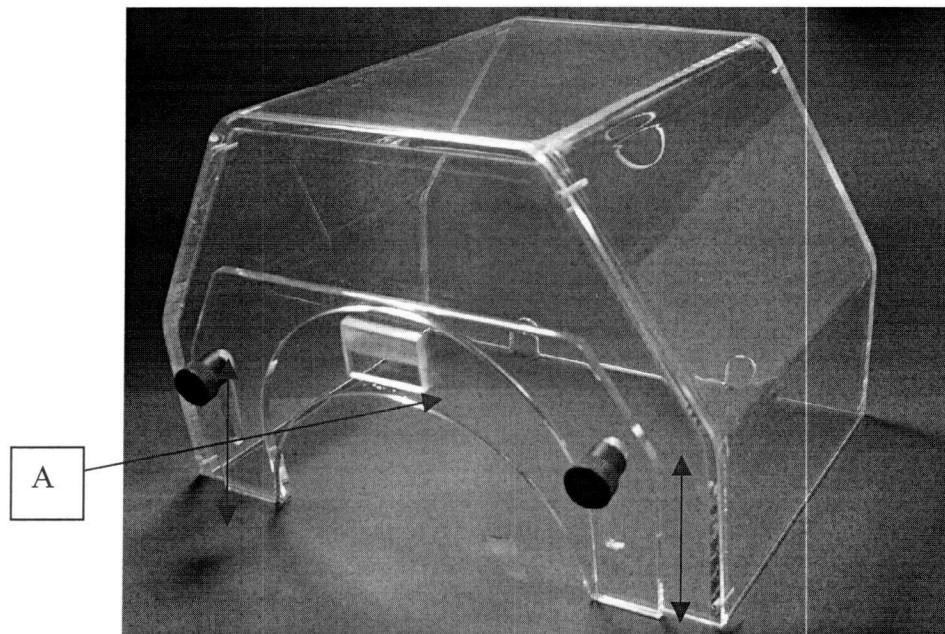

Adjust the height of the neck aperture (A) to reduce excessive gas and heat loss allowing the infants neck freedom of movement, and tighten screws to secure in place.

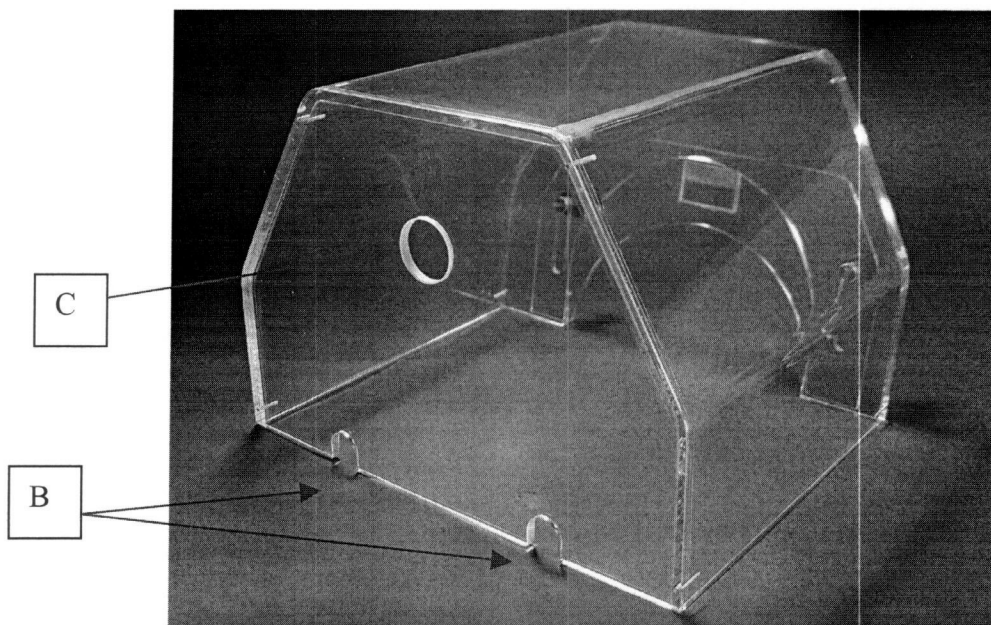

Use the access cutouts in the base (B) to run IV lines or oxygen sensor cables into the Head Box. The 22mm input hole (C) can be used to supply Oxygen via a standard oxygen tube 5mm or a humidified gas using 22mm or 15mm standard fittings

**Warning:**

Whilst using all types of Viamed Head boxes routinely check blood oxygen level to be certain of adequate carbon dioxide washout, use at least 6 litres a minute of air/oxygen mixture.

For babies weighing less than 1500 grams, the Viamed Head box should be pre-warmed to approximately 35 °C before placing over the infant. Either in the incubator or under a radiant warmer, placing a cold head box over a small baby may decrease body temperature as radiant losses from the baby can contribute to the warming of the oxygen hood.

It is recommended that the gas mixture be warmed and humidified before introduction.

Oxygen sensors should ideally be placed as near to the infant's mouth as possible

**Accessories:**

PP1968	Oxygen connector
PP1969	Diverter
PP1970	Special diverter
	Nascor Diverter
	Nascor soft neck seal
	Oxygen Analyser