

Medical Oxygen Sensors

The only source for all OEM and replacement respiratory and anesthesia O2 sensors



CE
0123



✓ Unmatched Quality Control

Every sensor is subjected to extensive quality assurance testing providing you with documented test results and the most reliable oxygen sensors available today. (See back page)

✓ Longest Expected Life

Our technology offers the longest life in the industry.

✓ Realistic Warranty

Sensors are warranted for up to 18 months based on 60-70% oxygen levels. Don't be misled! Get the facts!

✓ Superior Service

The most common products ship within 24 hours. Knowledgeable engineers and service representatives are trained and ready to assist.



Respiratory Sensors



PSR-11-60-08

Response Time: 6 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Analyzers/Monitors:
Sensidyne—1000-E



PSR-11-75-KE7

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Analyzers/Monitors:
Maxtec OM-25A, OM-25ME / OM-25MEL, MaxBlend, & Venturi System
OEM Ventilators:
Newport HT-70, e360, & e500



PSR-11-75-KE1

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Analyzers/Monitors:
Maxtec OM25A and Vapotherm Precision Flow



PSR-11-75-KE8

Response Time: 13 seconds
Expected Life in Air: 24 months
Warranty: 24 months
OEM Ventilators:
SLE 5000
(International Only)



PSR-11-75-KE2

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Ventilators:
Puritan Bennett 740
(older version)



PSR-11-75-KE9

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Analyzers/Monitors:
Carefusion / Viasys Bird Sentry Blender, Maxtec OM-25A & OM-25ME / OM-25MEL, and MaxBlend &



PSR-11-75-KE4

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Ventilators:
Carefusion Vela



PSR-11-75-KE10+

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Analyzers/Monitors:
Maxtec OMO2+A



PSR-11-75-KE6

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Ventilators:
SLE 2000
(International Only)



PSR-11-75-KE13-PB

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 24 months
OEM Ventilators: PB 760, 840, 980, 960, PB# 10097559



Analytical Industries Inc.

The Only Source for All Replacement O₂ Sensors

All O₂ sensors are manufactured in the U.S. under independently certified QA programs



PSR-11-917-J6

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 15 months
OEM Sensors:

Envitec OOM202-1 and
IT Gambert M-03



PSR-11-77

Response Time: 6 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Analyzers/Monitors:
Newport OM100,
Sechrist 650 Monitor, and
Teledyne 60T, 91, & 200



PSR-11-917-M

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Ventilators:
Siemens 300 & 900 Series,
Carefusion Avea & Sipap,
GE Ivent, Versamed eVent,
and Taema Ceasar



PSR-11-915-G

Response Time: 9 seconds
Expected Life in Air: 60 months
Warranty: 14 months
OEM Incubators:
Ohmeda Giraffe



PSR-11-917-M2

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Ventilators:
PB 840 & PB 760



PSR-11-915-2i

Response Time: 9 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Ventilators:
Drager Baby Log and
EVITA 2, 4, & XL SEMES
OEM Incubators:
Drager I800



PSR-11-917-MH

Response Time: 4 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Analyzers/Monitors:
Criticare Poet Monitor
OEM Ventilators:
Hamilton G5, Galileo,
Raphael, & Arabella



PSR-11-917-J

Response Time: 13 seconds
Expected Life in Air: 60 months
Warranty: 18 months
OEM Incubators:

MEDIX Natalcare
OEM Analyzers/Monitors:
MSA Mini Ox 1, 2, 3, & 3000,
Precision Medical PM5900,
PM5900L, & PB7820,
Teledyne AX 300 & MX 300, and
Takaoka KT 605
OEM Ventilators:
Philips Respironics Esprit & V200,
Stephan Christina, and
Taema Ceasar



PSR-11-917-MHJ

Response Time: 9 seconds
Expected Life in Air: 60 months
Warranty: 12 months
OEM Ventilators:
Biomed Device Cross Vents
w/ color display





✓ Unmatched Quality
✓ Longest Expected Life

✓ Realistic Warranty
✓ Superior Service



PSR-11-917-MH3

Response Time: 9 seconds

Expected Life in Air: 60 months

Warranty: 12 months

OEM Ventilators:

Biomed Device Cross Vents
w/ mono chrome black
display



All-11-60

Response Time: 13 seconds

Expected Life in Air: 60 months

Warranty: 18 months

OEM Analyzers/Monitors:

All-2000A & All-2000M



PSR-11-917-MH1

Response Time: 4 seconds

Expected Life in Air: 60 months

Warranty: 14 months

OEM Incubators:

Atom V-2100G & V-2200,
Drager C2000, and Drager /
Airshield Isolette w/ built-in



PSR-11-33

Response Time: 30 seconds

Expected Life in Air: 24 months

Warranty: 12 months

OEM Ventilators:

Hamilton Amadeus & Veolar



PSR-11-917-MH3

Response Time: 4 seconds

Expected Life in Air: 60 months

Warranty: 14 months

OEM Incubators:

Atom 100 Dual Incu I and
Atom 101 Dual Incu II



PSR-11-55

Response Time: 9 seconds

Expected Life in Air: 42 months

Warranty: 14 months

OEM Analyzers/Monitors:

Hudson 5577, 6477, & 5590



PSR-11-917-J1

Response Time: 13 seconds

Expected Life in Air: 60 months

Warranty: 18 months

OEM Analyzers/Monitors:

Maxtec OM-25A &
OM-25ME / OM-25MEL



PSR-11-58

Response Time: 13 seconds

Expected Life in Air: 60 months

Warranty: 18 months

OEM Analyzers/Monitors:

Hudson 5800 & 5801



PSR-11-77-CT4

Response Time: 13 seconds

Expected Life in Air: 60 months

Warranty: 14 months

OEM Sensor:

City Tech MOX-4



PSR-11-58HC

Response Time: 13 seconds

Expected Life in Air: 60 months

Warranty: 14 months

OEM Analyzers/Monitors:

Hudson RCI 5802



Anesthesia Sensors



PSR-11-915-4

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

GE / Datex Ohmeda 7900 &
7100 Smart Vent, Aestiva 300 /
5, Aespire, ADU w/ OEM Holder,
Avance w/ OEM Holder, and
Asys w/ OEM Holder



PSR-11-55HL

Response Time: 13 seconds

Warranty: 15 months

OEM Anesthesia Machines:

Heinen+Lowenstein Leon
Machine (Sold
internationally only)



PSR-11-60-03

Response Time: 13 seconds

Warranty: 14 months

OEM Analyzers/Monitors:

Penlon AVS & AV900

OEM Sensor:

City Tech MOX-3



PSR-11-915

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Ohmeda 4700 Oxicap, 5100
Series, 5250 RGM, 7200,
7800 Series, and Excel &
Modules Series



PSR-11-915-21

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Drager Cato, Fabuis w/ OEM
external cable, Narkomed
1A, 2, 2B, 3, & 4, Narkomed
6000 & 6400, and GS



PSR-11-917-J7

Response Time: 13 seconds

Warranty: 14 months

OEM Analyzers/Monitors:

Mindray A5, Wato EX-30 /
EX-20, EX-50 / EX-55, and
EX-60 / EX-65

OEM Sensor:

City Tech MOX-2



PSR-11-75-KE-250A

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Space Lab Blease and
Sirius Anesthesia Machine



PSR-11-77-CT4

Response Time: 13 seconds

Warranty: 14 months

OEM Sensor:

City Tech MOX-4



PSR-11-915-1

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Drager Narcomed Series,
6000, 6400, and Fabius w/
OEM External cable



Anesthesia Sensors Continued...



PSR-11-917-J3

Response Time: 13 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Datascope Anestar (new style) and Taema (France)
Alys & Clarys



PSR-11-917-J2

Response Time: 13 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Datascope Anestar (Older)



PSR-11-915-3

Response Time: 9 seconds

Warranty: 18 months

OEM Anesthesia Machines:

Ohmeda 5100, 5120, 5140,
5150, 7200, 7800, & 7810



PSR-11-917-J6


Response Time: 13 seconds

Warranty: 15 months

OEM Sensors:

✓ Unmatched Quality Control

...the organization continually improves the effectiveness of the quality system and takes action to eliminate the causes of nonconformities

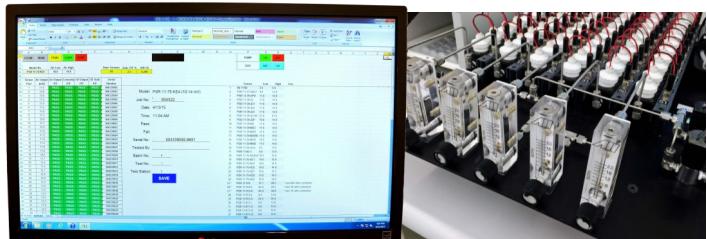

Following each critical operation in the assembly process, every sensor is tested to confirm signal output using equipment traceable to calibration certificates.

Once the assembly is complete, the critical performance parameters of every sensor are verified by an automated test protocol which generates two reports that identify both data points and PASS/FAIL test results as illustrated below and pictured left.

OLOS Automated mV Final Test Protocol

| 1 | | | | | |
|--------|--------------------|---------------|----------------------|-------------------|----------------------|
| Sensor | Output in Air (mV) | Output in Air | Linearity to 100% O2 | Output at 100% O2 | Stability at 100% O2 |
| 1 | 11.5 | PASS | PASS | PASS | PASS |
| 2 | 12.0 | PASS | PASS | PASS | PASS |
| 3 | 11.0 | PASS | PASS | PASS | PASS |
| 4 | 11.5 | PASS | PASS | PASS | PASS |
| 5 | 12.3 | PASS | PASS | PASS | PASS |

| 2 | Sensor (1-60) | Output in Air (mV) | Specification Test Parameters | | Stability over 100 Readings | | 1 | 99 | 100 |
|---|---------------|--------------------|-------------------------------|----------|-----------------------------|-------|------|------|-------|
| | | | Min Pass | Max Pass | Min | Max | | | |
| | 1 | 11.54 | 53.84 | 56.6 | 54.79 | 54.9 | PASS | PASS | 54.79 |
| | 2 | 12.01 | 56.02 | 58.9 | 57.25 | 57.33 | PASS | PASS | 57.27 |
| | 3 | 11.05 | 51.54 | 54.18 | 52.65 | 52.75 | PASS | PASS | 52.65 |
| | 4 | 11.55 | 53.87 | 56.64 | 55.17 | 55.25 | PASS | PASS | 55.17 |
| | 5 | 12.33 | 57.52 | 60.47 | 58.99 | 59.05 | PASS | PASS | 59.00 |

Serial numbers are assigned only to sensors that pass all aspects of the OLOS Final Test, thus establishing traceability.

By simulating operating conditions, the OLOS Final Test establishes documented confidence in the quality and performance of sensors accepted into inventory for shipment to customers.

Distributed by: