

# List of Private Label

**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

## Contents

|    |                                      |   |
|----|--------------------------------------|---|
| 1  | List of Sensors .....                | 2 |
| 2  | Änderungsregister / Change log ..... | 2 |
| 3  | R- 23V (OOM201) .....                | 3 |
| 4  | R- 30V (OOM110) .....                | 3 |
| 5  | R- 41V (OOM202-1) .....              | 4 |
| 6  | R- 42V (OOM202-2S).....              | 4 |
| 7  | R- 43V (OOM112) .....                | 5 |
| 8  | R- 44V (OOM202-2) .....              | 5 |
| 9  | R- 45V (OOM106) .....                | 6 |
| 10 | R- 46V (OOM111).....                 | 6 |
| 11 | R-47V (OOM204).....                  | 7 |
| 12 | R-49V (OOM202).....                  | 7 |
| 13 | R- 22MEDV (OOM103).....              | 8 |
| 14 | R- 48V (OOM113).....                 | 8 |
| 15 | R- 15V (OOM101).....                 | 9 |
| 16 | Customer Approval .....              | 9 |

|                                                                                                                                     |                                |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|--------------------------------|------------------|
|                                                  | Created –<br>Erstellt:         | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | <b>ML</b><br><b>06.09.2017</b> | <b>1 / 9</b>     |

# List of Private Label

**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

## 1 List of Sensors

| No. | EnviteC Sensor - Type | Viamed PN = EnviteC Order Ref. | Envitec Article number | Final model number |
|-----|-----------------------|--------------------------------|------------------------|--------------------|
| 1   | OOM201                | 0110023                        | 01-00-0014             | R- 23V             |
| 2   | OOM110                | 0110040                        | 01-00-0098             | R- 30V             |
| 3   | OOM202-1              | 0110041                        | 01-00-0021             | R- 41V             |
| 4   | OOM202-2S             | 0110042                        | 1000106                | R- 42V             |
| 5   | OOM112                | 0110043                        | 1001202                | R- 43V             |
| 6   | OOM202-2              | 0110044                        | 01-00-0068             | R- 44V             |
| 7   | OOM106                | 0110045                        | 01-00-0091             | R- 45V             |
| 8   | OOM111                | 0110046                        | 01-00-0114             | R- 46V             |
| 9   | OOM204                | 0110047                        | 01-00-0097             | R- 47V             |
| 10  | OOM202                | 0110049                        | 01-00-0047             | R- 49V             |
| 11  | OOM103                | 0110021                        | 01-00-0015             | R- 22MEDV          |
| 12  | OOM113                | 0110048                        | 1002178                | R-48V              |
| 13  | OOM101                | 0110014                        | 01-00-0013             | R-15V              |

## 2 Änderungsregister / Change log

| Revision | Date       | Author                  | Description                                                                                                                       |
|----------|------------|-------------------------|-----------------------------------------------------------------------------------------------------------------------------------|
| 0        | 10.12.2014 | Maik Lingies            | New document design data from document "Private Label VIAMED_update_2013-07-16" and add the Sensor type OOM202, OOM204 and OOM113 |
| 1        | 25.09.2015 | Steffen Wickner         | Anpassung des Labeldesign nach Anforderungen des DCR550 von Viamed                                                                |
| 2        | 28.10.2015 | Steffen Wickner         | Change of the Prefix of the serial number from Z to V on request of Viamed                                                        |
| 3        | 14.09.2016 | Christian von Walsleben | Change Blister Label accordance to UDI standart                                                                                   |
| 4        | 06.09.2017 | Maik Lingies            | Add new Sensor RV-15V                                                                                                             |

|                                                                                                                                   |                                |               |
|-----------------------------------------------------------------------------------------------------------------------------------|--------------------------------|---------------|
|                                                | Created – Erstellt:            | Page – Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Navigation\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | <b>ML</b><br><b>06.09.2017</b> | <b>2 / 9</b>  |

# List of Private Label


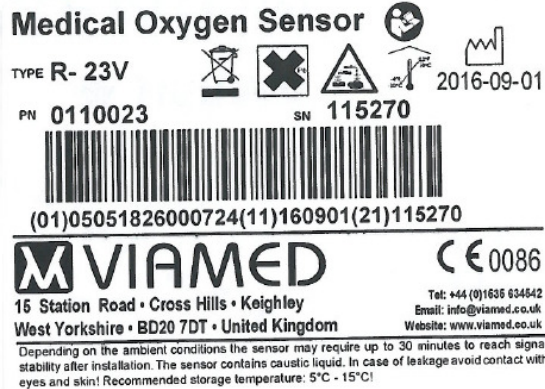
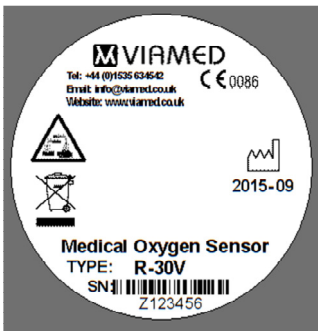
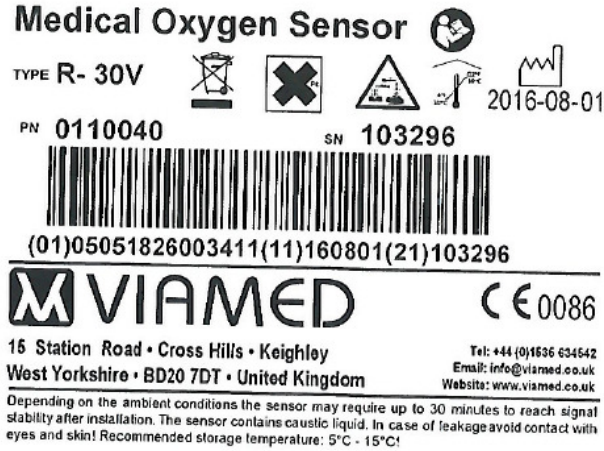
**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 3 R- 23V (OOM201)                                                                   |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|    |    |
| 4 R- 30V (OOM110)                                                                   |                                                                                      |
| Label on Sensor (dia. 39,8)                                                         | Label on Blister- Card (63,5x46,6)                                                   |
|  |  |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 3 / 9            |

# List of Private Label


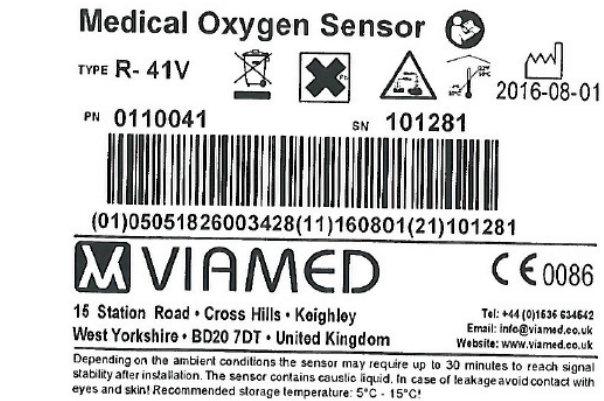


**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 5 R- 41V (OOM202-1)                                                                                                                                                                                                                                                     |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Label on Sensor (90x11)                                                                                                                                                                                                                                                 | Label on Blister- Card (63,5x46,6)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|  <p>VIAMED Medical Oxygen Sensor<br/>Tel: +44 (0)1535 634542<br/>Email: info@viamed.co.uk<br/>Website: www.viamed.co.uk<br/>CE 0086<br/>TYPE: R- 41V<br/>SN: Z123456<br/>2015-09</p>   |  <p>Medical Oxygen Sensor<br/>TYPE R- 41V<br/>PN 0110041 SN 101281<br/>(01)05051826003428(11)160801(21)101281<br/>VIAMED CE 0086<br/>16 Station Road • Cross Hills • Keighley<br/>West Yorkshire • BD20 7DT • United Kingdom<br/>Tel: +44 (0)1636 634642<br/>Email: info@viamed.co.uk<br/>Website: www.viamed.co.uk<br/>Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!</p> |
| 6 R- 42V (OOM202-2S)                                                                                                                                                                                                                                                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| Label on Sensor (90x11)                                                                                                                                                                                                                                                 |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|  <p>VIAMED Medical Oxygen Sensor<br/>Tel: +44 (0)1535 634542<br/>Email: info@viamed.co.uk<br/>Website: www.viamed.co.uk<br/>CE 0086<br/>TYPE: R- 42V<br/>SN: Z123456<br/>2015-09</p> |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| Label on plastic container (90x11)                                                                                                                                                                                                                                      |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|  <p>VIAMED Medical Oxygen Sensor<br/>Tel: +44 (0)1535 634542<br/>Email: info@viamed.co.uk<br/>Website: www.viamed.co.uk<br/>CE 0086<br/>TYPE: R- 42V<br/>SN: Z123456<br/>2015-09</p> |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 4 / 9            |

# List of Private Label


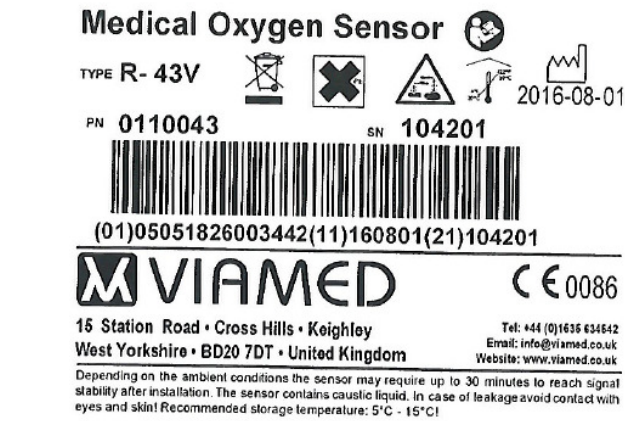

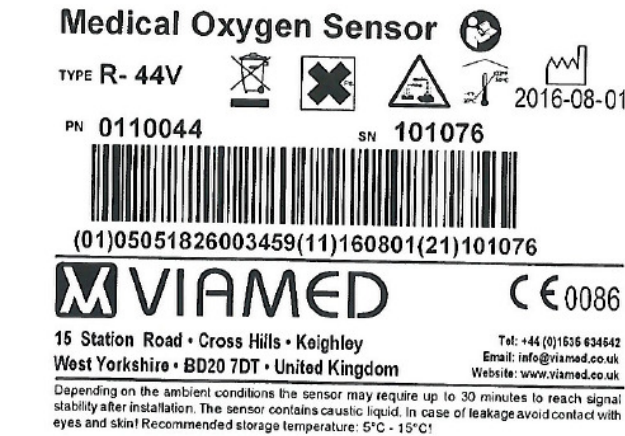
**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 7 R- 43V (OOM112)                                                                   |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| Label on Sensor (90x15)                                                             | Label on single Blister- Card (pack of 2)<br>(63,5x46,6)                             |
|    |   |
| 8 R- 44V (OOM202-2)                                                                 |                                                                                      |
| Label on Sensor (90x11)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|  |  |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 5 / 9            |

# List of Private Label


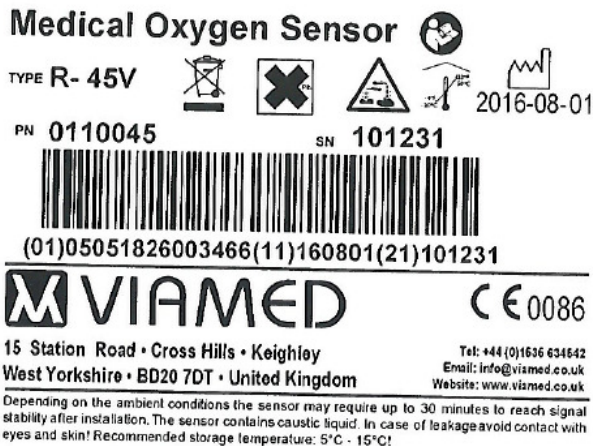

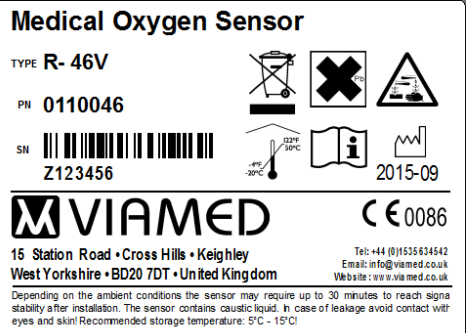
**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 9 R- 45V (OOM106)                                                                   |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| Label on Sensor (90x11)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|    |   |
| 10 R- 46V (OOM111)                                                                  |                                                                                      |
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|  |  |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 6 / 9            |



# List of Private Label


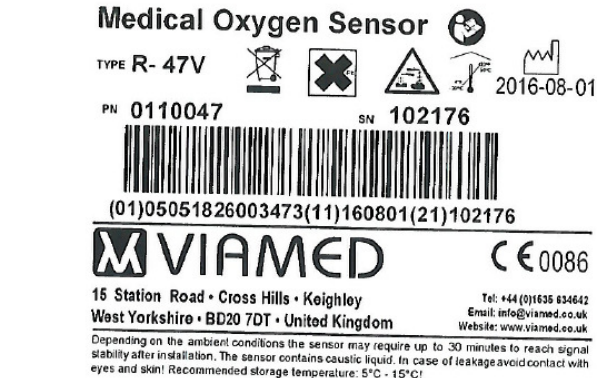

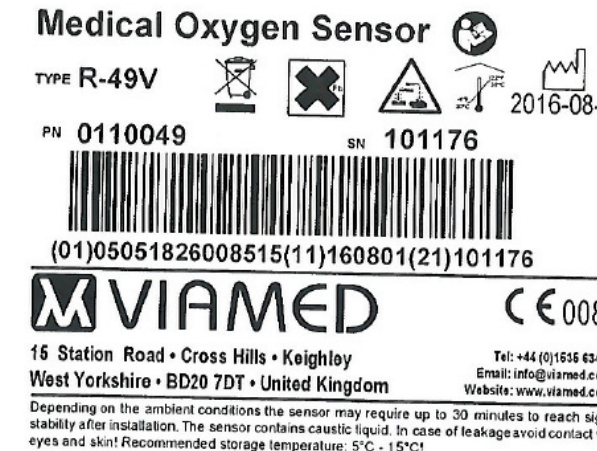
**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 11 R-47V (OOM204)                                                                   |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|    |    |
| 12 R-49V (OOM202)                                                                   |                                                                                      |
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|  |  |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 7 / 9            |

# List of Private Label

**Honeywell**


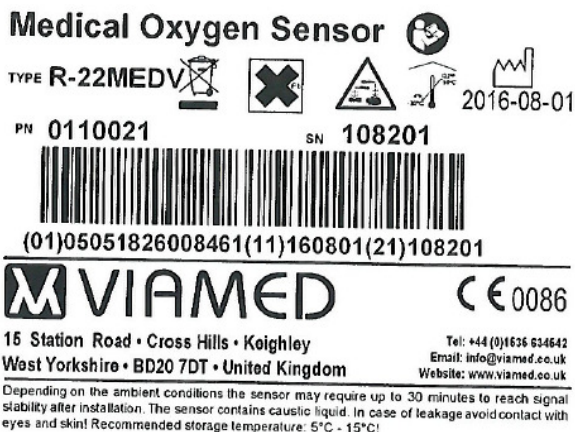

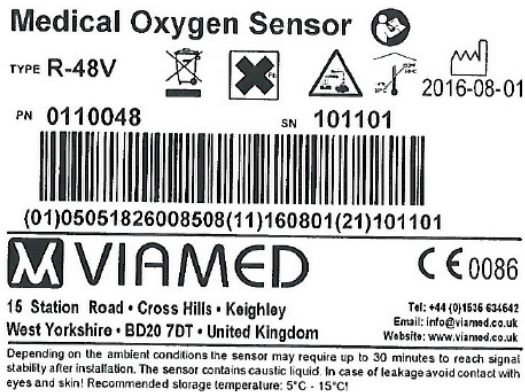
**Customer: VIAMED**

**ENVITEC**

by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 13 R- 22MEDV (OOM103)                                                               |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|    |   |
| 14 R- 48V (OOM113)                                                                  |                                                                                      |
| Label on Sensor (90x15)                                                             | Label on Blister- Card (63,5x46,6)                                                   |
|  |  |

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 8 / 9            |



# List of Private Label


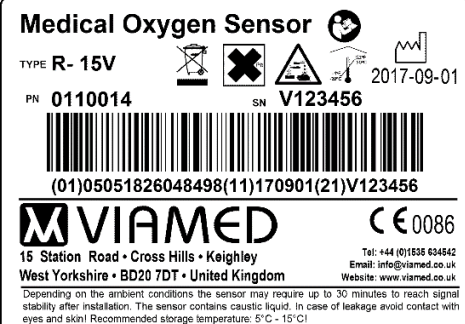
**Honeywell**

**Customer: VIAMED**

**ENVITEC**  
by Honeywell

**Confidential!**

For use by EnviteC and VIAMED only!

| 15 R- 15V (OOM101)                                                                                                                                              |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Label on Sensor (90x15)                                                                                                                                         | Label on Blister- Card (63,5x46,6)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|  <p>VIAMED Medical Oxygen Sensor<br/>TYPE: R- 15V SN: Z123456<br/>2017- 09</p> |  <p>Medical Oxygen Sensor<br/>TYPE R- 15V<br/>PN 0110014 SN V123456<br/>2017-09-01<br/>(01)05051826048498(11)170901(21)V123456<br/>VIAMED<br/>15 Station Road • Cross Hills • Keighley<br/>West Yorkshire • BD20 7DT • United Kingdom<br/>Tel: +44 (0)1838 634642<br/>Email: info@viamed.co.uk<br/>Website: www.viamed.co.uk<br/>CE0086<br/>Depending on the ambient conditions the sensor may require up to 30 minutes to reach signal stability after installation. The sensor contains caustic liquid. In case of leakage avoid contact with eyes and skin! Recommended storage temperature: 5°C - 15°C!</p> |

## 16 Customer Approval

Date:

Signature:

|                                                                                                                                     |                        |                  |
|-------------------------------------------------------------------------------------------------------------------------------------|------------------------|------------------|
|                                                  | Created –<br>Erstellt: | Page –<br>Seite: |
| \\Ge0ynt004307\produkte\PRODUKT.001\PHA\Fertigungsunterlagen\Label_Na<br>vision\Viamed\Freigaben\001-29-Private_Label_VIAMED-4.docx | ML<br>06.09.2017       | 9 / 9            |