

VIAMED

Suppliers of Electromedical Equipment

2022



Wain Wath Force on the River Swale, Keld, Yorkshire Dales

January

M	31	3	10	17	24
T		4	11	18	25
W		5	12	19	26
T		6	13	20	27
F		7	14	21	28
S	1	8	15	22	29
S	2	9	16	23	30

February

M		7	14	21	28
T	1	8	15	22	
W	2	9	16	23	
T	3	10	17	24	
F	4	11	18	25	
S	5	12	19	26	
S	6	13	20	27	

March

M		7	14	21	28
T	1	8	15	22	29
W	2	9	16	23	30
T	3	10	17	24	31
F	4	11	18	25	
S	5	12	19	26	
S	6	13	20	27	

April

M		4	11	18	25
T		5	12	19	26
W		6	13	20	27
T		7	14	21	28
F	1	8	15	22	29
S	2	9	16	23	30
S	3	10	17	24	

May

M	30	2	9	16	23
T	31	3	10	17	24
W		4	11	18	25
T		5	12	19	26
F		6	13	20	27
S		7	14	21	28
S	1	8	15	22	29

June

M		6	13	20	27
T		7	14	21	28
W	1	8	15	22	29
T	2	9	16	23	30
F	3	10	17	24	
S	4	11	18	25	
S	5	12	19	26	

July

M		4	11	18	25
T		5	12	19	26
W		6	13	20	27
T		7	14	21	28
F	1	8	15	22	29
S	2	9	16	23	30
S	3	10	17	24	31

August

M	1	8	15	22	29
T	2	9	16	23	30
W	3	10	17	24	31
T	4	11	18	25	
F	5	12	19	26	
S	6	13	20	27	
S	7	14	21	28	

September

M		5	12	19	26
T		6	13	20	27
W		7	14	21	28
T	1	8	15	22	29
F	2	9	16	23	30
S	3	10	17	24	
S	4	11	18	25	

October

M	31	3	10	17	24
T		4	11	18	25
W		5	12	19	26
T		6	13	20	27
F		7	14	21	28
S	1	8	15	22	29
S	2	9	16	23	30

November

M		7	14	21	28
T	1	8	15	22	29
W	2	9	16	23	30
T	3	10	17	24	
F	4	11	18	25	
S	5	12	19	26	
S	6	13	20	27	

December

M		5	12	19	26
T		6	13	20	27
W		7	14	21	28
T	1	8	15	22	29
F	2	9	16	23	30
S	3	10	17	24	31
S	4	11	18	25	



VIAMED




15 Station Road · Cross Hills · Keighley · West Yorkshire · BD20 7DT · UK
Tel: +44 (0)1535 634 542 · Fax: +44 (0)1535 635 582
info@viamed.co.uk · www.viamed.co.uk



TOF^{3D} Neuromuscular Transmission Monitor

Quantitatively monitors the level of neuromuscular transmission during surgery or in the intensive care unit, as a means of assessing the depth or degree of muscle relaxation

- Reliable
- Easy to use
- Economical, uses standard low cost ECG electrodes
- Twitch response measured by accelerometer
- Displayed values
- Downloadable trend data

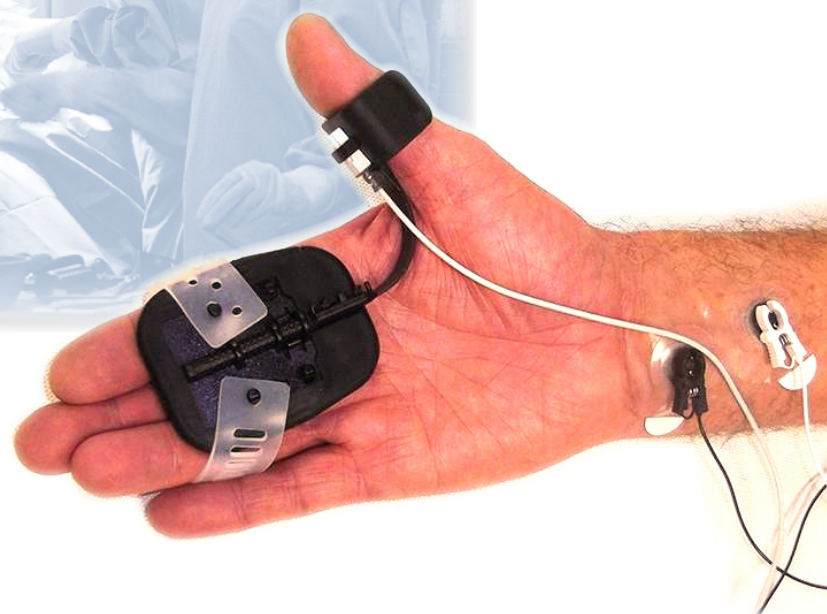





TOF^{3D} Neuromuscular
Transmission Monitor
REF: 2510091

By means of 3 dimensional acceleromyography (AMG), the TOF^{3D} quantitatively monitors the level of neuromuscular transmission during surgery or in the intensive care unit.

The new TOF^{3D} is easy to use and, in addition to the standard TOF and PTC modes, there are alternative objective and subjective modes of stimulation available.

The monitor's functions and modes of stimulation can be quickly customised to meet your specific requirements.

- **TOF - Train of Four**
Single stimulation or continuous every 15 seconds.
- **PTC - Post Tetanic Count**
- **TOFs - Train of Four**
Stimulation interval between 1 minute to 60 minutes.
- **Single Twitch** - 1Hz or 0.1Hz - Single stimulation or continuous.
- **DBS - Double Burst Stimulation** - Ratio 3-2 or 3-3.
- **TET** - Tetanic - 50 Hz or 100 Hz.

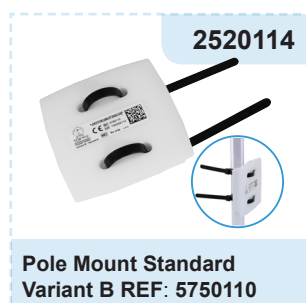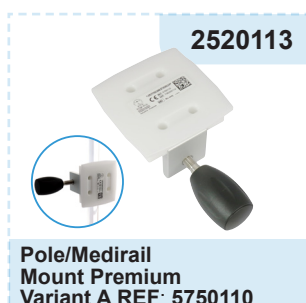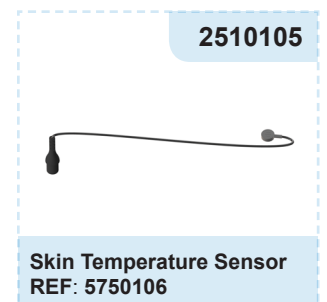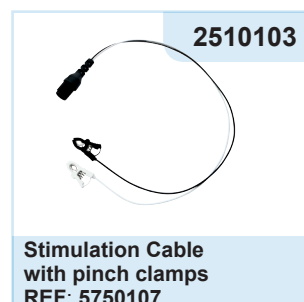

Accessories marked with a dotted border are NOT included as standard. Specifications subject to change