

VIAMED

Suppliers of Electromedical Equipment

2025

Winskill Stones, Langcliffe, Yorkshire Dales

January

M	6	13	20	27
T	7	14	21	28
W	1	8	15	22 28
T	2	9	16	23 30
F	3	10	17	24 31
S	4	11	18	25
S	5	12	19	26

February

M	3	10	17	24
T	4	11	18	25
W	5	12	19	26
T	6	13	20	27
F	7	14	21	28
S	1	8	15	22
S	2	9	16	23

March

M	31	3	10	17	24
T	4	11	18	25	
W	5	12	19	26	
T	6	13	20	27	
F	7	14	21	28	
S	1	8	15	22	29
S	2	9	16	23	30

April

M	7	14	21	28
T	1	8	15	22 29
W	2	9	16	23 30
T	3	10	17	24
F	4	11	18	25
S	5	12	19	26
S	6	13	20	27

May

M	5	12	19	26
T	6	13	20	27
W	7	14	21	28
T	1	8	15	22 29
F	2	9	16	23 30
S	3	10	17	24 31
S	4	11	18	25

June

M	30	2	9	16	23
T	3	10	17	24	
W	4	11	18	25	
T	5	12	19	26	
F	6	13	20	27	
S	7	14	21	28	
S	1	8	15	22	29

July

M	7	14	21	28
T	1	8	15	22 29
W	2	9	16	23 30
T	3	10	17	24 31
F	4	11	18	25
S	5	12	19	26
S	6	13	20	27

August

M	4	11	18	25
T	5	12	19	26
W	6	13	20	27
T	7	14	21	28
F	1	8	15	22 29
S	2	9	16	23 30
S	3	10	17	24 31

September

M	1	8	15	22	29
T	2	9	16	23	30
W	3	10	17	24	
T	4	11	18	25	
F	5	12	19	26	
S	6	13	20	27	
S	7	14	21	28	

October

M	6	13	20	27
T	7	14	21	28
W	1	8	15	22 29
T	2	9	16	23 30
F	3	10	17	24 31
S	4	11	18	25
S	5	12	19	26

November

M	3	10	17	24
T	4	11	18	25
W	5	12	19	26
T	6	13	20	27
F	7	14	21	28
S	1	8	15	22 29
S	2	9	16	23 30

December

M	1	8	15	22	29
T	2	9	16	23	30
W	3	10	17	24	31
T	4	11	18	25	
F	5	12	19	26	
S	6	13	20	27	
S	7	14	21	28	



VIAMED

15 Station Road · Cross Hills · Keighley · West Yorkshire · BD20 7DT · UK
Tel: +44 (0)1535 634 542 · Fax: +44 (0)1535 635 582
info@viamed.co.uk · www.viamed.co.uk



Medical Gas Sensors



Significant savings can be made by switching to Viamed.
See Viamed's comprehensive range of OEM and compatible Oxygen Sensors at


www.viamed.co.uk/xref

Viamed continue to provide a gas sensor disposal service as part of our
Waste Management Policy, contact us for further details or order your bags online at

www.viamed.co.uk/disposal

Disposable EEG Sensors

for monitoring the depth of anaesthesia as well as acquisition
and transmission of biological EEG signals

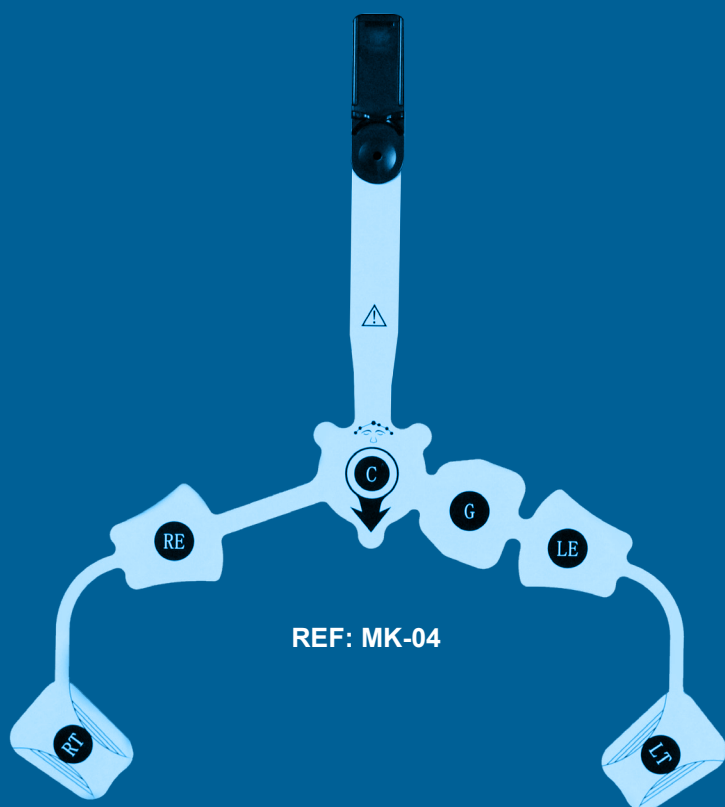

REF: MK-04




REF: MK-01



REF: MK-02



REF: MK-03

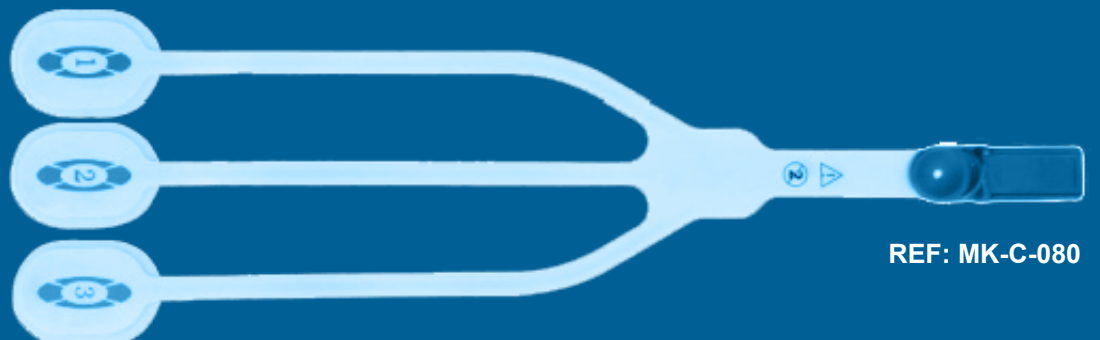

REF: MK-C-080



VIAMED

Tel: 01535 634 542

Specifications Subject to Change
Part Number: 0196000