

VIAMED

Suppliers of Electromedical Equipment

2025



Winskill Stones, Langcliffe, Yorkshire Dales

January

M		6	13	20	27
T		7	14	21	28
W	1	8	15	22	28
T	2	9	16	23	30
F	3	10	17	24	31
S	4	11	18	25	
S	5	12	19	26	

February

M		3	10	17	24
T		4	11	18	25
W		5	12	19	26
T		6	13	20	27
F		7	14	21	28
S	1	8	15	22	
S	2	9	16	23	

March

M	31	3	10	17	24
T		4	11	18	25
W		5	12	19	26
T		6	13	20	27
F		7	14	21	28
S	1	8	15	22	29
S	2	9	16	23	30

April

M		7	14	21	28
T	1	8	15	22	29
W	2	9	16	23	30
T	3	10	17	24	
F	4	11	18	25	
S	5	12	19	26	
S	6	13	20	27	

May

M		5	12	19	26
T		6	13	20	27
W		7	14	21	28
T	1	8	15	22	29
F	2	9	16	23	30
S	3	10	17	24	31
S	4	11	18	25	

June

M	30	2	9	16	23
T		3	10	17	24
W		4	11	18	25
T		5	12	19	26
F		6	13	20	27
S		7	14	21	28
S	1	8	15	22	29

July

M		7	14	21	28
T	1	8	15	22	29
W	2	9	16	23	30
T	3	10	17	24	31
F	4	11	18	25	
S	5	12	19	26	
S	6	13	20	27	

August

M		4	11	18	25
T		5	12	19	26
W		6	13	20	27
T		7	14	21	28
F	1	8	15	22	29
S	2	9	16	23	30
S	3	10	17	24	31

September

M	1	8	15	22	29
T	2	9	16	23	30
W	3	10	17	24	
T	4	11	18	25	
F	5	12	19	26	
S	6	13	20	27	
S	7	14	21	28	

October

M		6	13	20	27
T		7	14	21	28
W	1	8	15	22	29
T	2	9	16	23	30
F	3	10	17	24	31
S	4	11	18	25	
S	5	12	19	26	

November

M		3	10	17	24
T		4	11	18	25
W		5	12	19	26
T		6	13	20	27
F		7	14	21	28
S	1	8	15	22	29
S	2	9	16	23	30

December

M	1	8	15	22	29
T	2	9	16	23	30
W	3	10	17	24	31
T	4	11	18	25	
F	5	12	19	26	
S	6	13	20	27	
S	7	14	21	28	



VIAMED

15 Station Road · Cross Hills · Keighley · West Yorkshire · BD20 7DT · UK
Tel: +44 (0)1535 634 542 · Fax: +44 (0)1535 635 582
info@viamed.co.uk · www.viamed.co.uk





The Leading Medical Gas Sensors Supplier

Maximise Savings with Viamed's range of Medical Gas Sensors

Significant savings can be made by switching to Viamed.

See Viamed's comprehensive range of OEM and compatible Oxygen Sensors at

www.viamed.co.uk/xref

FREE Gas Sensor Disposal - Simplify Your Waste Management Today


Viamed continue to provide a FREE gas sensor disposal service as part of our Waste Management Policy, contact us for further details or order your bags online at

www.viamed.co.uk/disposal




VIAMED Tel: 01535 634 542

Specifications Subject to Change
Part Number: 0196000

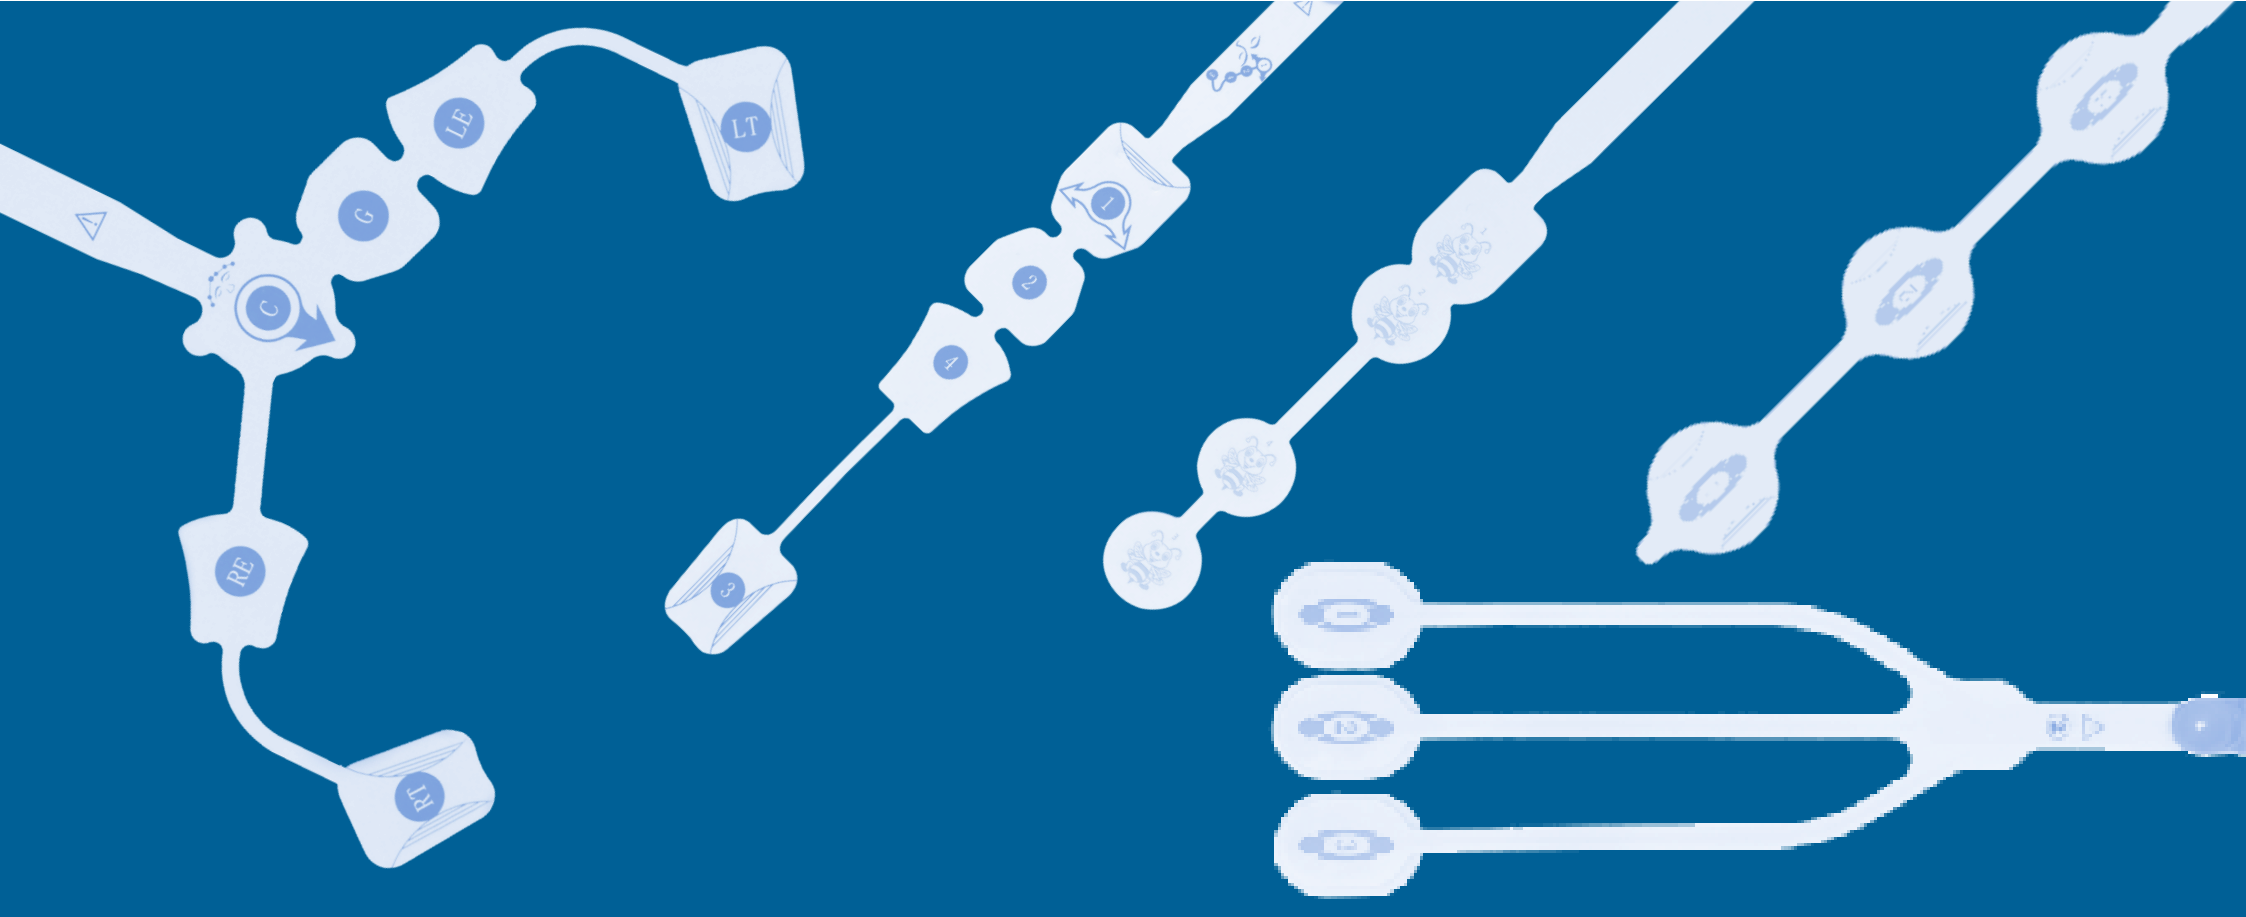

Disposable EEG Sensors

For monitoring the depth of anaesthesia as well as acquisition and transmission of biological EEG signals

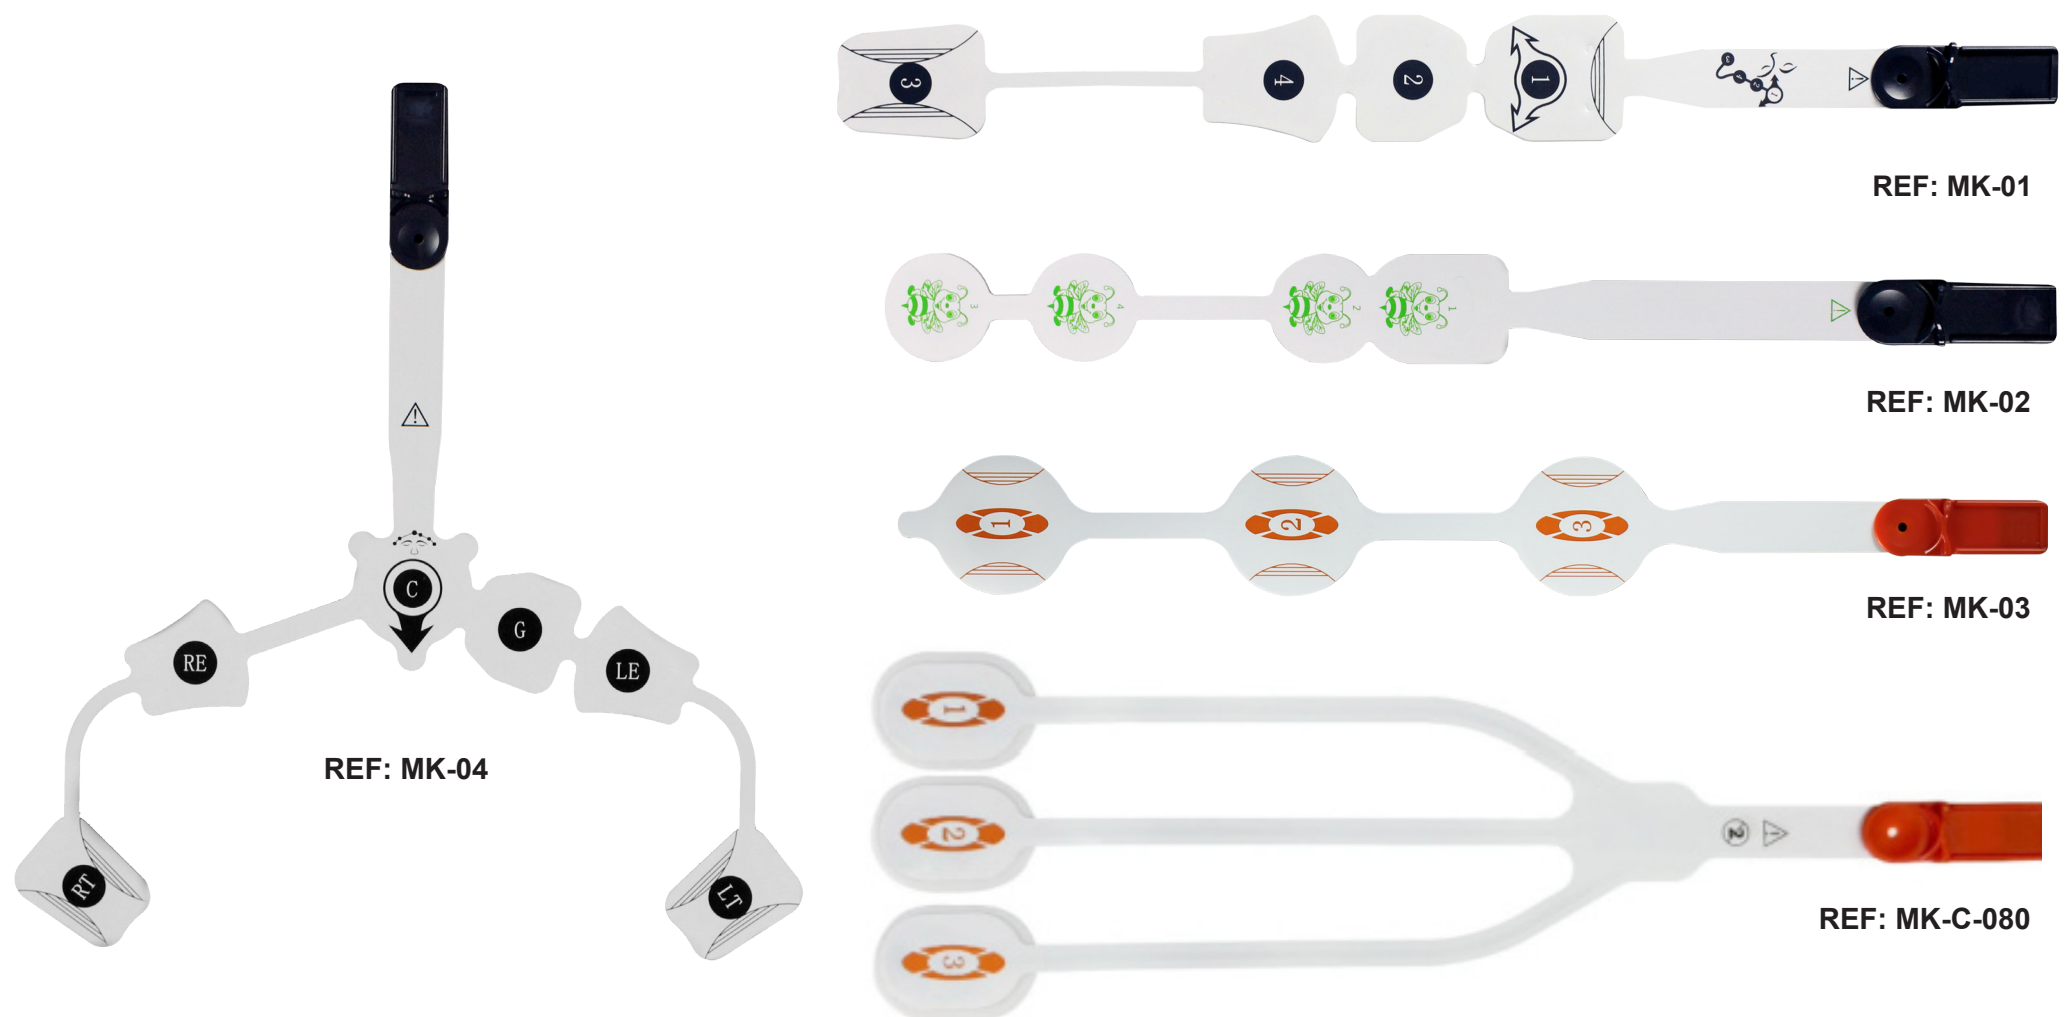

- BIS EEG sensors compatible with a wide range of BIS™ monitors and modules
- GE Entropy Compatible
- Clinically tested, high-measurement accuracy
- Soft and bio-compatible material
- Latex-free



VIAMED Tel: 01535 634 542

Specifications Subject to Change
Part Number: 0196000