
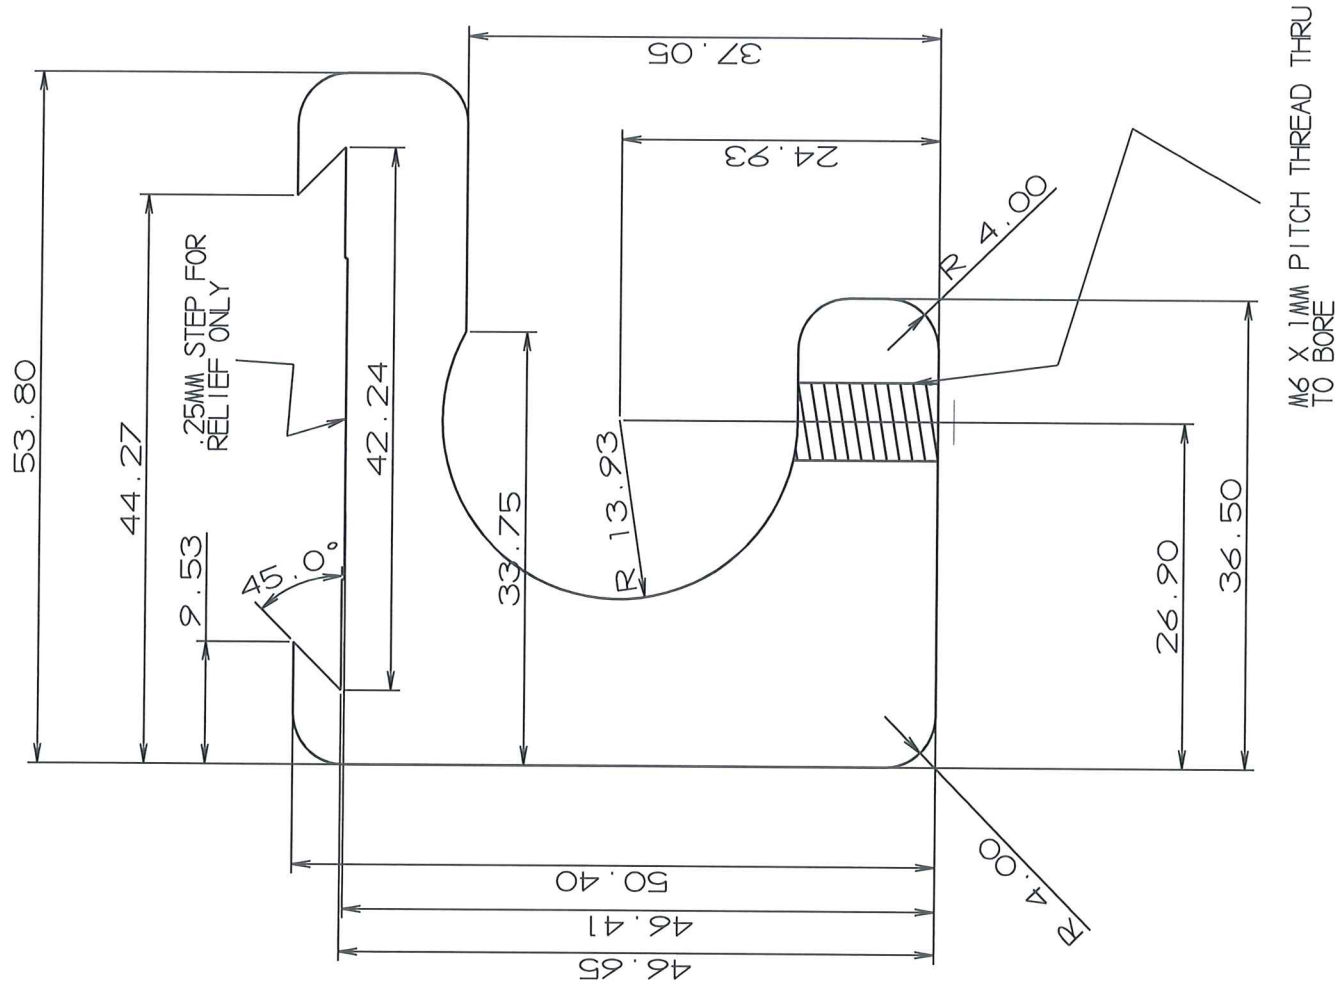


CONTROLLED ISSUE	
ISSUE NO <u>7</u>	DATE <u>31/12/12</u>
AUTH <u>MAR</u>	

A4781
 DRAWN M. GARNER 2-10-12
 VIAMED CONTACT STEVE NIXON
 01535 634 542

NOTE
 DIMENSIONS FOR
 TAPER ARE APPROX
 AND MUST FIT ALL PLASTIC
 COMPONENTS SUPPLIED
 BY VIAMED
 ANY QUESTIONS PLEASE ASK.

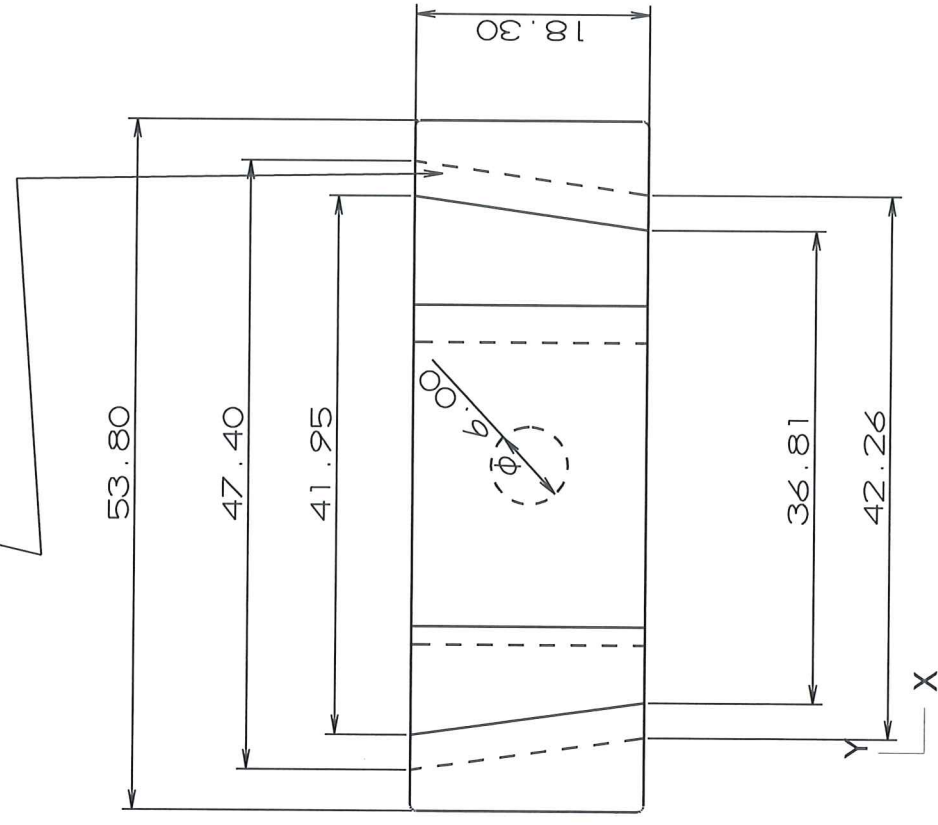

M6 X 1MM PITCH THREAD THRU
 TO BORE

mm