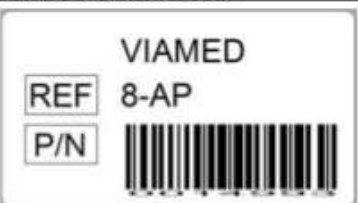


	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 1 of 6

1. SPO2 sensor group: **Viamed Disposable sensors**
 ➤ Example: **8-AP, Disposable sensor for adults**

Compatibility sensor label	Label appearance
Content a) Name of manufacturer b) Compatibility information	 For use with VIAMED oximeters only
Pouch Label	Label appearance
Content a) Identification of packed sensor in English, French, German and Spain b) Quantity of packed sensors in English, French, German and Spain c) Compatibility information in English, French, German and Spain d) Symbol for user manual e) Symbol for single use f) Symbol for latex free materials g) Symbol for disposal h) Name and address of medical product manufacturer i) CE mark and Body number of medical product manufacturer j) REF information k) LOT information l) Usability information	
Box side label	Label appearance
Content a) Compatibility information b) REF information c) P/N information	

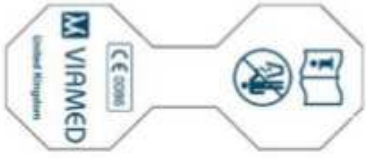
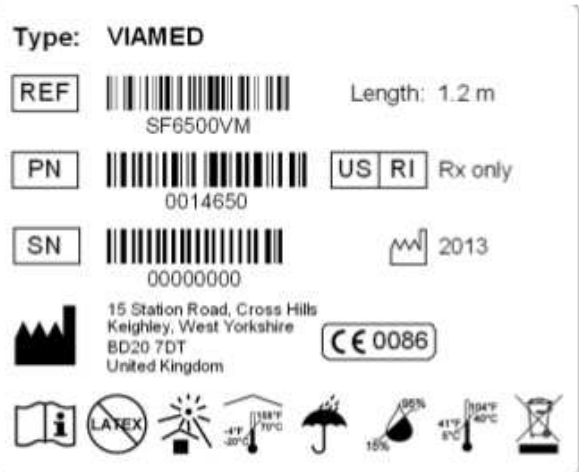
Created: R. Dettweiler Date: 13/18/10	Approved: Ralf Dettweiler Date: 13/18/10
File:Z:\Entwicklung\Project_SpO2_Sensors\PHA_SPO2_Sensors\PHA_SPO2-S_3.Produkt dokumentation\3.5.GA_Inserts_Labeling\Labeling\Viamed\Viamed_Labeling_SPO2 sensors_Rev.0.doc	

	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 2 of 6

Box top label	Label appearance
Content a) Sensor identification b) Compatibility information c) Sensor length information d) REF information e) Packaging quantity f) P/N information g) Usability information h) LOT information i) Advise for US market j) Name and address of medical product manufacturer k) CE mark and Body number of medical product manufacturer l) Symbol for user manual m) Symbol for latex free materials n) Symbol for single use o) Symbol of light protection p) Symbol of storage temperature range q) Symbol "keep dry" r) Symbol of humidity range s) Symbol for usage temperature range t) Symbol for disposal	

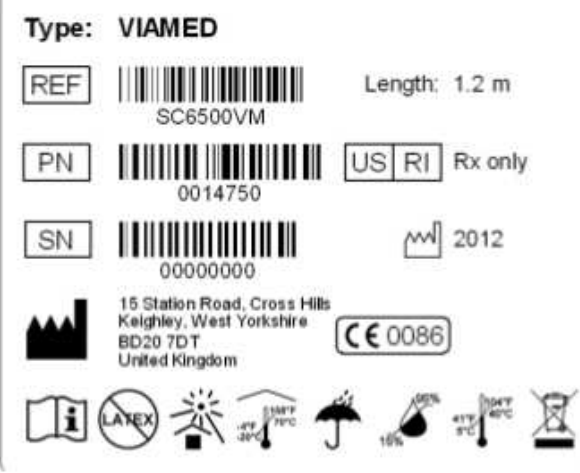
	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 3 of 6

2. SPO2 sensor group: Viamed Finger clip sensors
 ➤ Example: SF6500VM

Compatibility sensor label	Label appearance
Content a) Name of manufacturer b) Compatibility information	
Serial number sensor label	Label appearance
Content a) REF information b) Serial number	
Manufacturer sensor label	Label appearance
Content a) Viamed Logo b) Viamed CE mark with body number c) Symbol for disposal d) Symbol for user manual	
Box side label	Label appearance
Content a) Compatibility information b) REF information c) P/N information	
Box top label	Label appearance
Content a) Compatibility information b) REF information c) Sensor length information d) P/N information e) Advise for US market f) S/N information g) Year of manufacturing h) Address of medical product manufacturer i) CE mark and Body number of medical product manufacturer j) Symbol for user manual k) Symbol for latex free materials l) Symbol of light protection m) Symbol of storage temperature range n) Symbol "keep dry" o) Symbol of humidity range p) Symbol for usage temperature range q) Disposal information	

	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 4 of 6

3. SPO2 sensor group: Viamed Soft sensors
 ➤ Example: SC6500VM

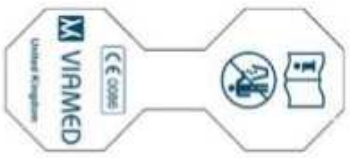
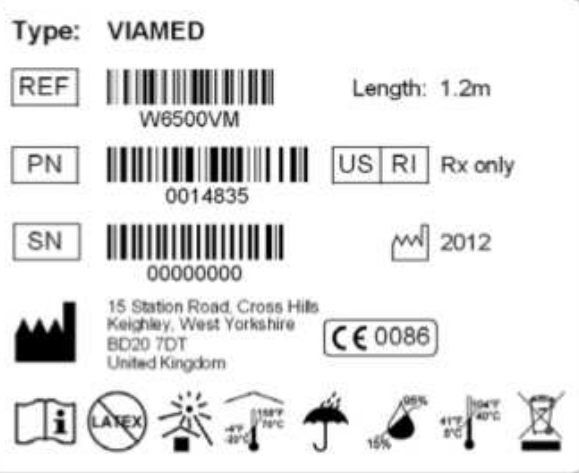
Compatibility sensor label	Label appearance
Content a) Name of manufacturer b) Compatibility information	
Serial number sensor label	Label appearance
Content a) REF information b) Serial number	
Manufacturer sensor label	Label appearance
Content a) Viamed Logo b) Viamed CE mark with body number c) Symbol for disposal d) Symbol for user manual	
Box side label	Label appearance
Content a) Compatibility information b) REF information c) P/N information	
Box top label	Label appearance
Content a) Compatibility information b) REF information c) Sensor length information d) P/N information e) Advise for US market f) S/N information g) Year of manufacturing h) Address of medical product manufacturer i) CE mark and Body number of medical product manufacturer j) Symbol for user manual k) Symbol for latex free materials l) Symbol of light protection m) Symbol of storage temperature range n) Symbol "keep dry" o) Symbol of humidity range p) Symbol for usage temperature range q) Disposal information	

	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 5 of 6

4. SPO2 sensor group:

➤ Example:

**Viamed Wrap sensors
W6500VM**

Compatibility sensor label	Label appearance
Content a) Name of manufacturer b) Compatibility information	
Serial number sensor label	Label appearance
Content a) REF information b) Serial number	
Manufacturer sensor label	Label appearance
Content a) Viamed Logo b) Viamed CE mark with body number c) Symbol for disposal d) Symbol for user manual	
Box side label	Label appearance
Content a) Compatibility information b) REF information c) P/N information	
Box top label	Label appearance
Content a) Compatibility information b) REF information c) Sensor length information d) P/N information e) Advise for US market f) S/N information g) Year of manufacturing h) Address of medical product manufacturer i) CE mark and Body number of medical product manufacturer j) Symbol for user manual k) Symbol for latex free materials l) Symbol of light protection m) Symbol of storage temperature range n) Symbol "keep dry" o) Symbol of humidity range p) Symbol for usage temperature range q) Disposal information	

	Viamed	Revision 0
Internal Document	Labelling SPO2 sensors	Page 6 of 6

5. SPO2 sensor group:

➤ Example:

**Viamed Ear sensors
EP6500VM**

Compatibility sensor label	Label appearance
Content a) Name of manufacturer b) Compatibility information	
Serial number sensor label	Label appearance
Content a) REF information b) Serial number	
Manufacturer sensor label	Label appearance
Content a) Viamed Logo b) Viamed CE mark with body number c) Symbol for disposal d) Symbol for user manual	
Box side label	Label appearance
Content a) Compatibility information b) REF information c) P/N information	
Box top label	Label appearance
Content a) Compatibility information b) REF information c) Sensor length information d) P/N information e) Advise for US market f) S/N information g) Year of manufacturing h) Address of medical product manufacturer i) CE mark and Body number of medical product manufacturer j) Symbol for user manual k) Symbol for latex free materials l) Symbol of light protection m) Symbol of storage temperature range n) Symbol "keep dry" o) Symbol of humidity range p) Symbol for usage temperature range q) Disposal information	