

	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 1 von 14

Issued	Signature	Date
Rayk Jürgensen		
Reviewed	Signature	Date
Approved	Signature	Date
Bernd Lindner		

Document History Log

Rev.	Date / By	Modifications
0	25.10.2012 / SB	Initial version
1	10.12.2013 / RJ	Complete sampling accessories
2	01.07.2015 / RJ	Updated date and rev. on label

Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 2 von 14


1. Label Layout: CO2 Sampling lines

Dimension Inlay: 105 mm x 100 mm


Dimension Box Label: 68 mm x 99 mm

Ref.: 4420560

CO2 Single Port Nasal Sampling Prong

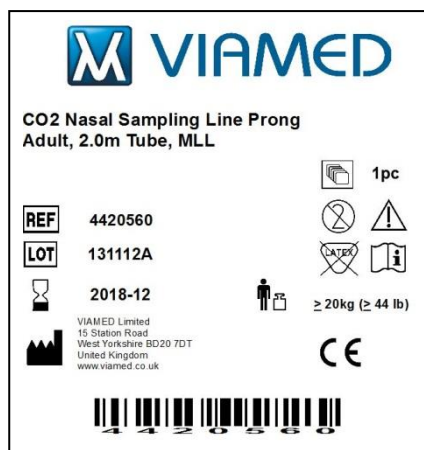


Front view

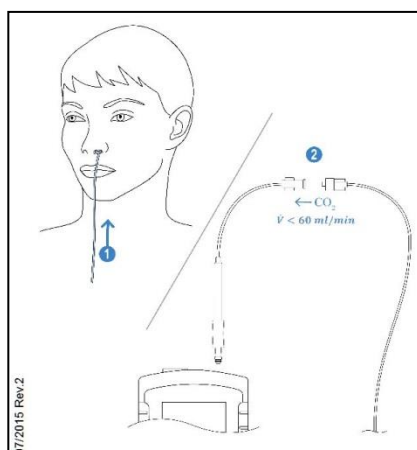

Rear view

Box Label

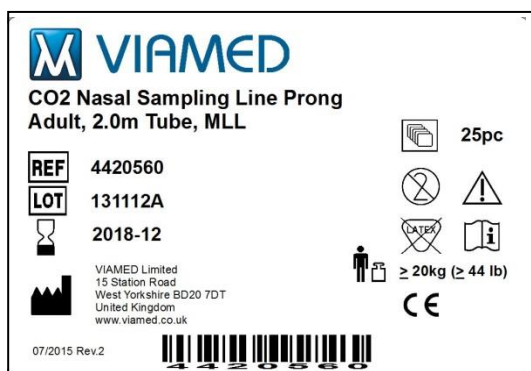

Erstellt: R. Jürgensen

Datum: 2015-07-01


Datei: Viamed_Labeling_gas sampling accessories_rev2

Freigabe: R.Jürgensen


Datum: 2015-07-01

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 3 von 14

Ref.: 4420710
Nasal Sampling Line, Adult

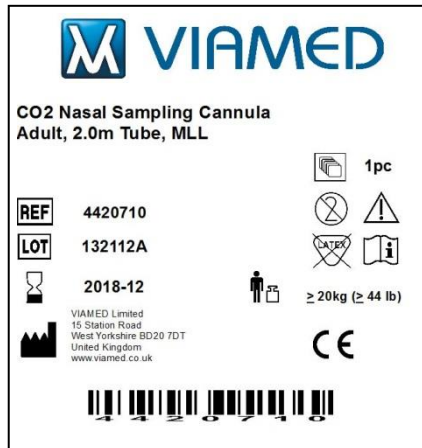


Front view

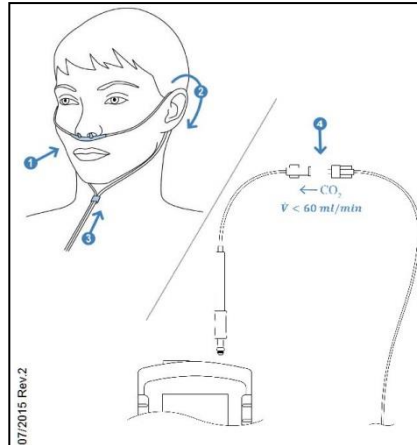

Rear view


Box Label

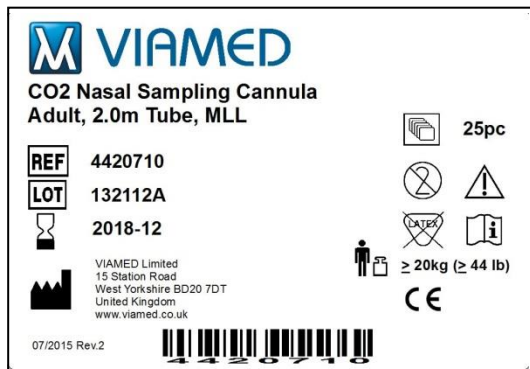


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 4 von 14

Ref.: 4420711
Nasal Sampling Line, Pediatric

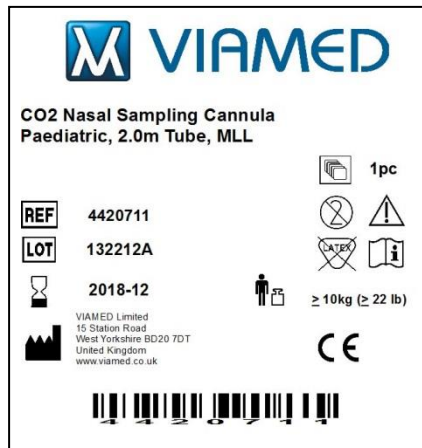


Front view

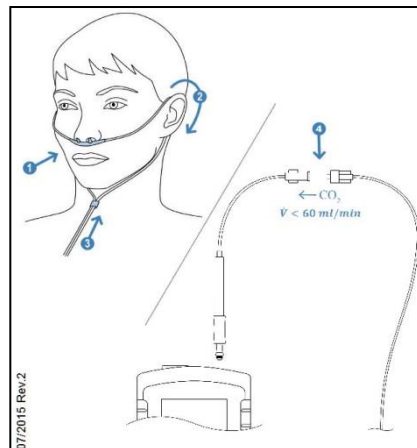

Rear view


Box Label

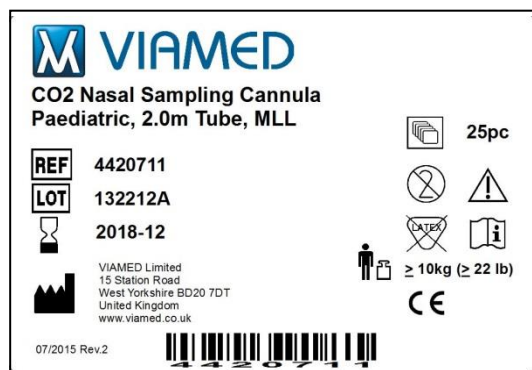


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 5 von 14

Ref.: 4420713
Nasal Sampling Line, Infant

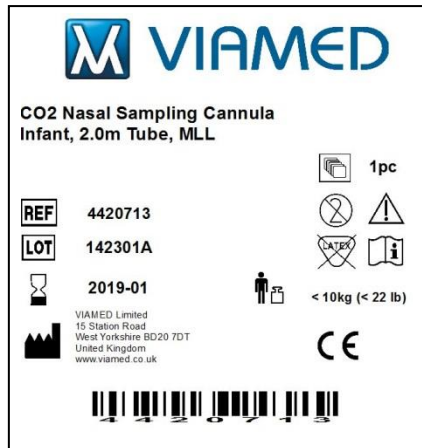


Front view

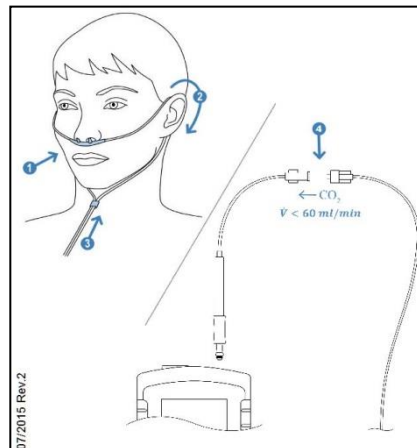

Rear view

Box Label

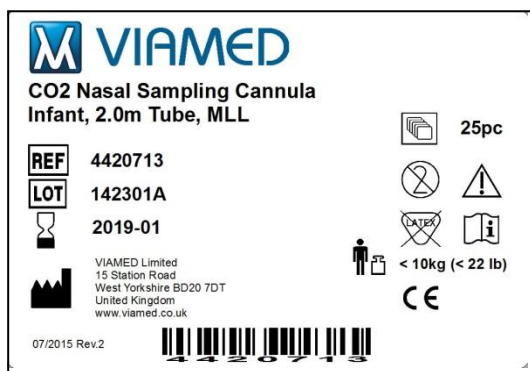


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 6 von 14

Ref.: 4420718

Nasal Sampling Line with O2 Supply, Adult

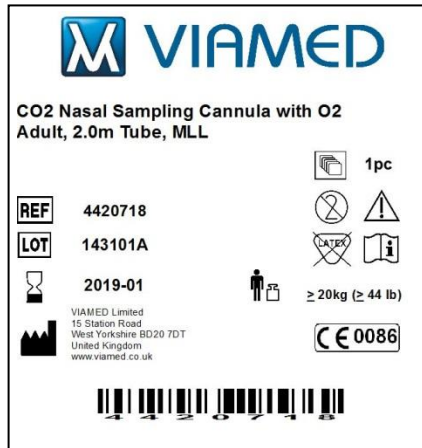


Front view

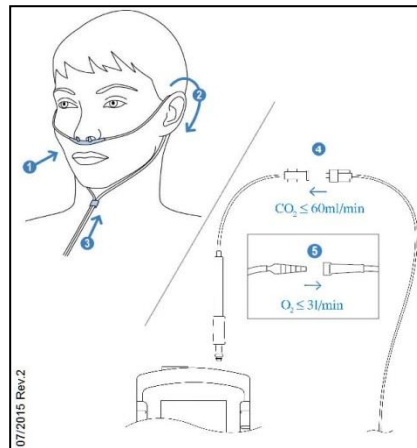

Rear view


Box Label

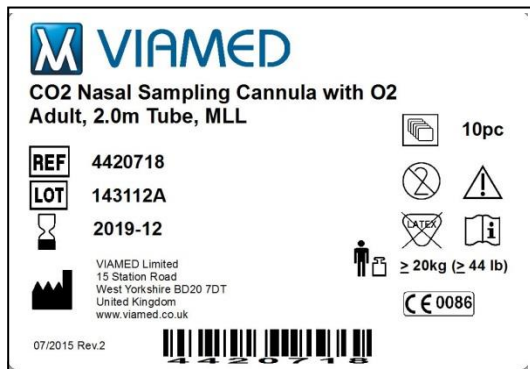


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 7 von 14

Ref.: 4420719
Nasal Sampling Line with O2 Supply, Pediatric

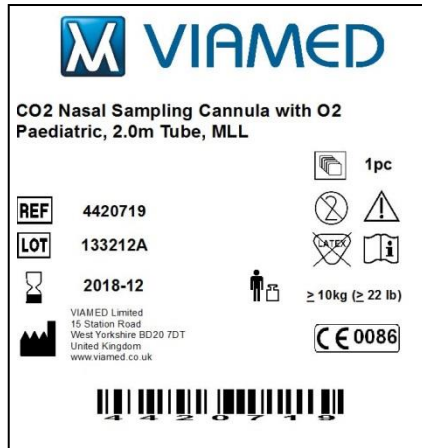


Front view

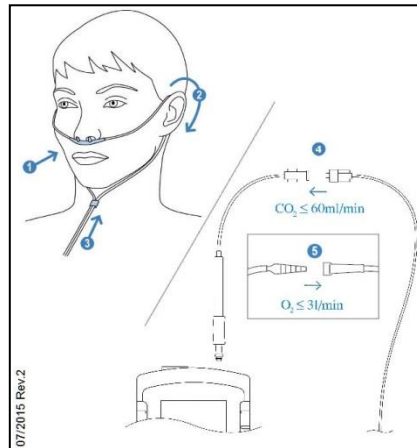

Rear view

Box Label

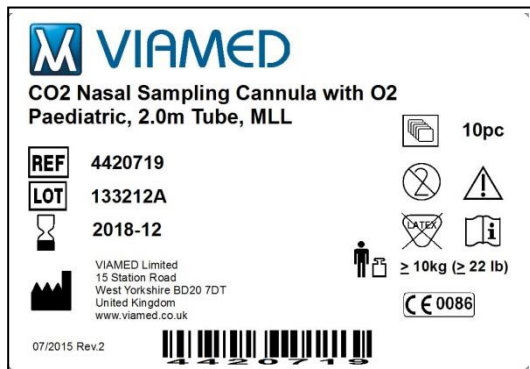


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 8 von 14

Ref.: 4420730

Oral/Nasal Sampling Line, Adult

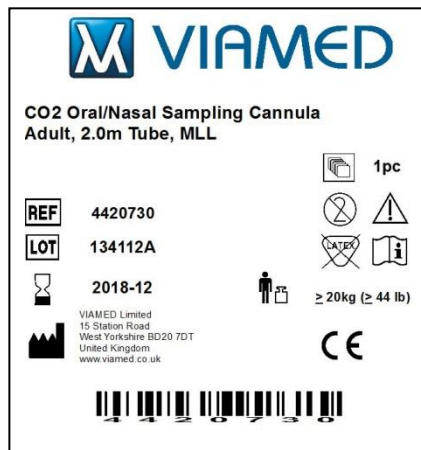


Front view

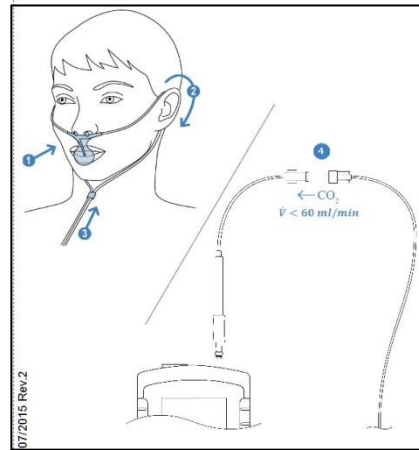

Rear view

Box Label

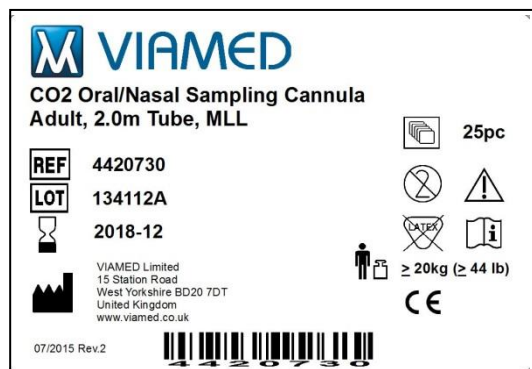


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 9 von 14

Ref.: 4420731

Oral/Nasal Sampling Line, Pediatric

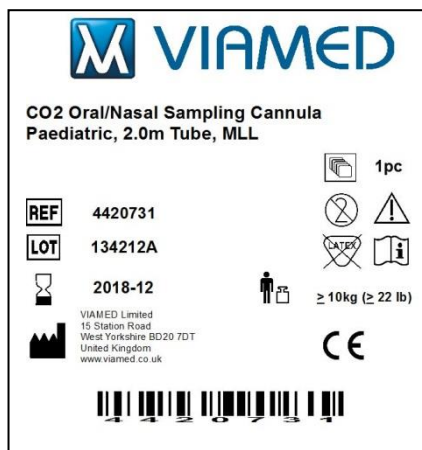


Front view

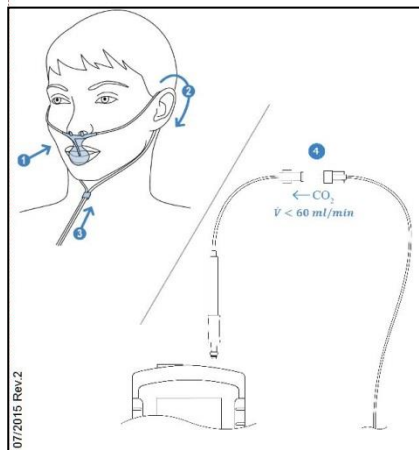

Rear view

Box Label

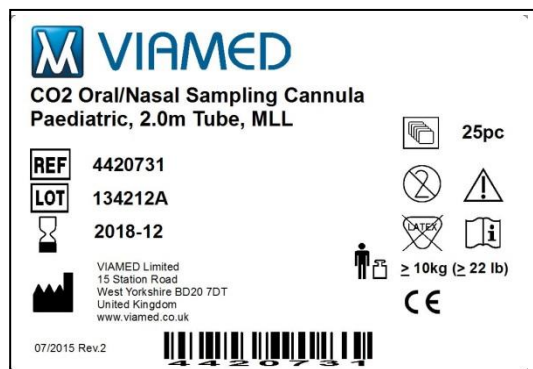


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 10 von 14

Ref.: 4420738

Oral/Nasal Sampling Line with O2 Supply, Adult

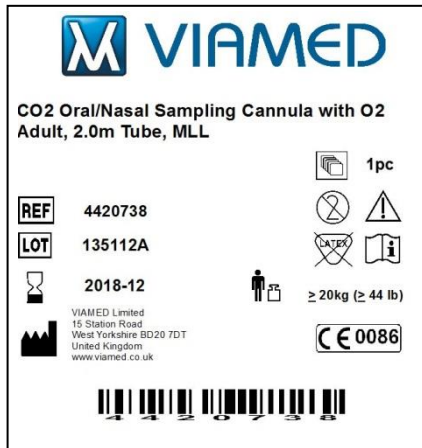


Front view

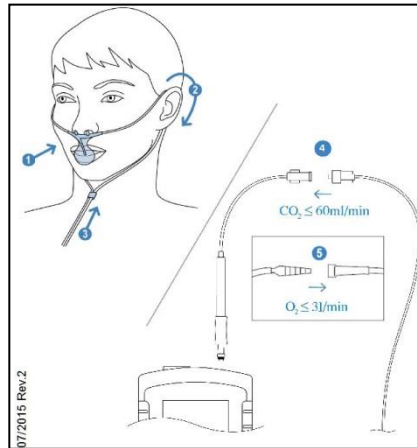

Rear view

Box Label

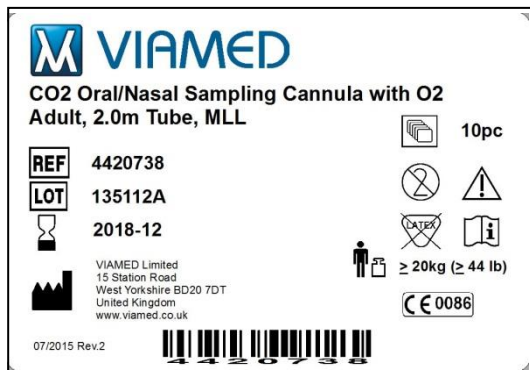


Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R. Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 11 von 14

Ref.: 4420739

Oral/Nasal Sampling Line with O2 Supply, Pediatric

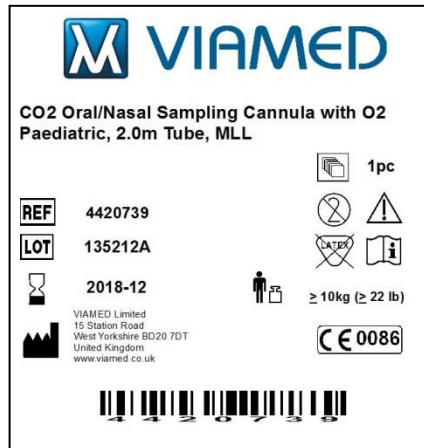


Front view

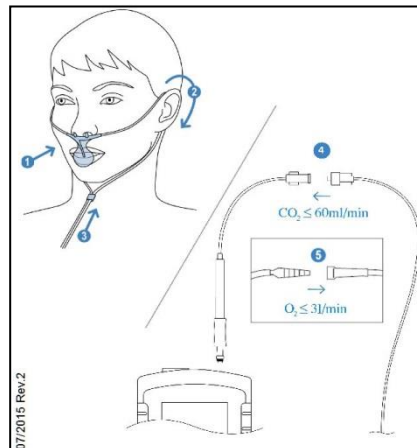

Rear view


Box Label

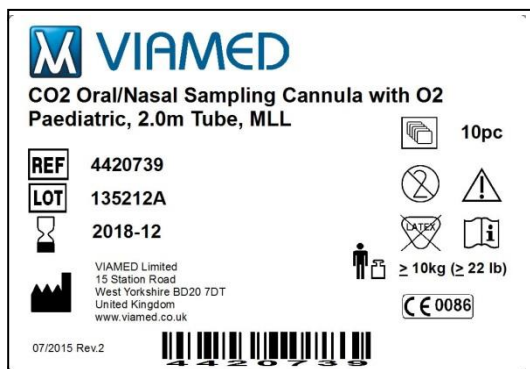

Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R. Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 12 von 14

Tag Layout:

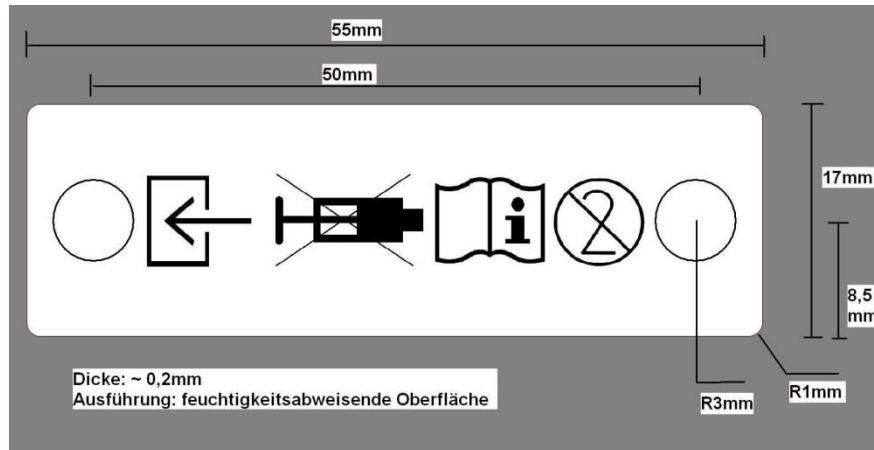

Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	


bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 13 von 14

2. Label Layout: Nomo Adapter

Dimension: 70 mm x 37 mm

Ref.: 4420525

Nomo Adapter

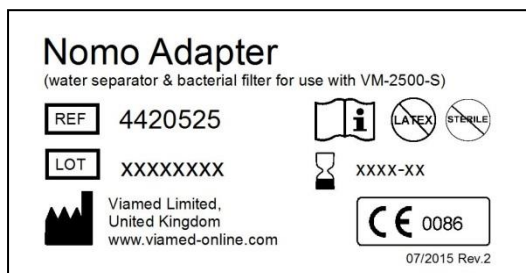

3. Label Layout: Sampling lines

Dimension Single Label: 38 mm x 21 mm

Dimension Box Label: 68 mm x 99 mm


Ref.: 4420551

Disposable sampling line, Single



Ref.: 4420550

Disposable sampling line, Box

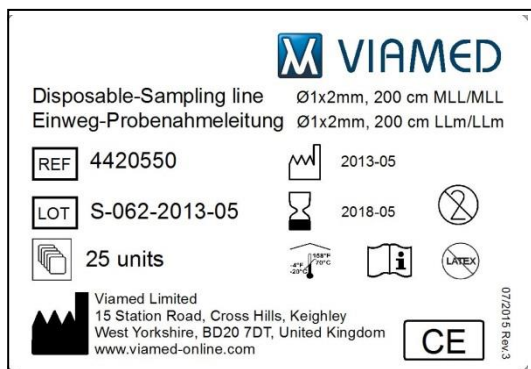

Erstellt: R. Jürgensen

Datum: 2015-07-01

Freigabe: R.Jürgensen

Datum: 2015-07-01

Datei: Viamed_Labeling_gas sampling accessories_rev2

bluepoint MEDICAL	PHA Gas Sampling Accessorie	Revision 2
Internal Document	Viamed Labeling	Seite 14 von 14

4. Label Layout: Airway Adapter

Dimension Single Label: 38 mm x 21 mm

Dimension Box Label: 68 mm x 99 mm

Ref.: 4420531

Disposable sampling line, Single

Sidestream airway adapter (Adult/Paediatric)				
REF	4420531			07/2015 Rev.1
LOT	01102010			
www.viamed-online.com				

Box Label:

	
Sidestream airway adapter - Adult/Paediatric (Accessorie for VM-2500-S)	
REF 4420531	 25 units
LOT 01102010	  
 Viamed Limited 15 Station Road, Cross Hills, Keighley West Yorkshire, BD20 7DT, United Kingdom www.viamed-online.com	
CE 0088	
07/2015 Rev.3	

Erstellt: R. Jürgensen Datum: 2015-07-01	Freigabe: R.Jürgensen Datum: 2015-07-01
Datei: Viamed_Labeling_gas sampling accessories_rev2	