

Operator's Manual

V1000 Foetal Heart Simulator



Manufactured by:

Viamed Ltd.
15 Station Road
Cross Hills
Keighley
West Yorkshire, BD20 7DT
United Kingdom

Tel: +44 (0)1535 634542
Fax: +44 (0)1535 635582
E-mail: info@viamed.co.uk
Website: www.viamed.co.uk

Distributed by:

This publication is protected by copyright and all rights are reserved. No part of this manual may be reproduced or transmitted in any form or by any means electronic or mechanical, including photocopying and recording for any purpose other than the purchasers personal use, without the written permission of Viamed Ltd. Information within this document is subject to change. Changes will be made without notice and incorporated in further issues. V1000 is a registered trademark of Viamed Ltd., who recognise all trademarks and products of manufacturers mentioned.

© Copyright 2014 Viamed Ltd.

Contents

Section	Page
Introduction	4
Controls and Indicators	5
Operating the V1000	6
Low Battery Indication	7
Replacing the Batteries	7
Cleaning	8
Protection Rating	8
Warranty	8
V1000 Service Sheet	9

Introduction

The V1000 Foetal Heart Simulator allows the operation of foetal heart monitors to be verified and the accuracy of displayed foetal heart rate assessed.

It is a hand held, portable unit for use in any environment where foetal heart monitors need to be tested: before use, when suspected faulty or after routine servicing.

The V1000 simulates heart rates in the range of 30 BPM to 210 BPM.

Altering the intensity control on the front panel alters the amplitude, allowing the sensitivity of the transducer and monitor combination to be assessed.

The V1000 can simulate continuously in excess of 2 weeks at maximum intensity, using 4 x 1.5V AA/MN1500/LR6 alkaline batteries.

Areas of Application for the V1000

The following is a breakdown of when the V1000 can be used:

By Engineers for:

Fault finding and diagnosis of the monitor

Soak testing of the monitor

As part of a Planned Preventative Maintenance procedure

Verification of correct chart paper installed

By Midwives & Clinicians for:


Testing the foetal heart monitors and transducers prior to use

Verification of correct chart paper installed

For Teaching purposes:

Simulation of the foetal heart and training in the use of monitoring equipment

Controls and Indicators

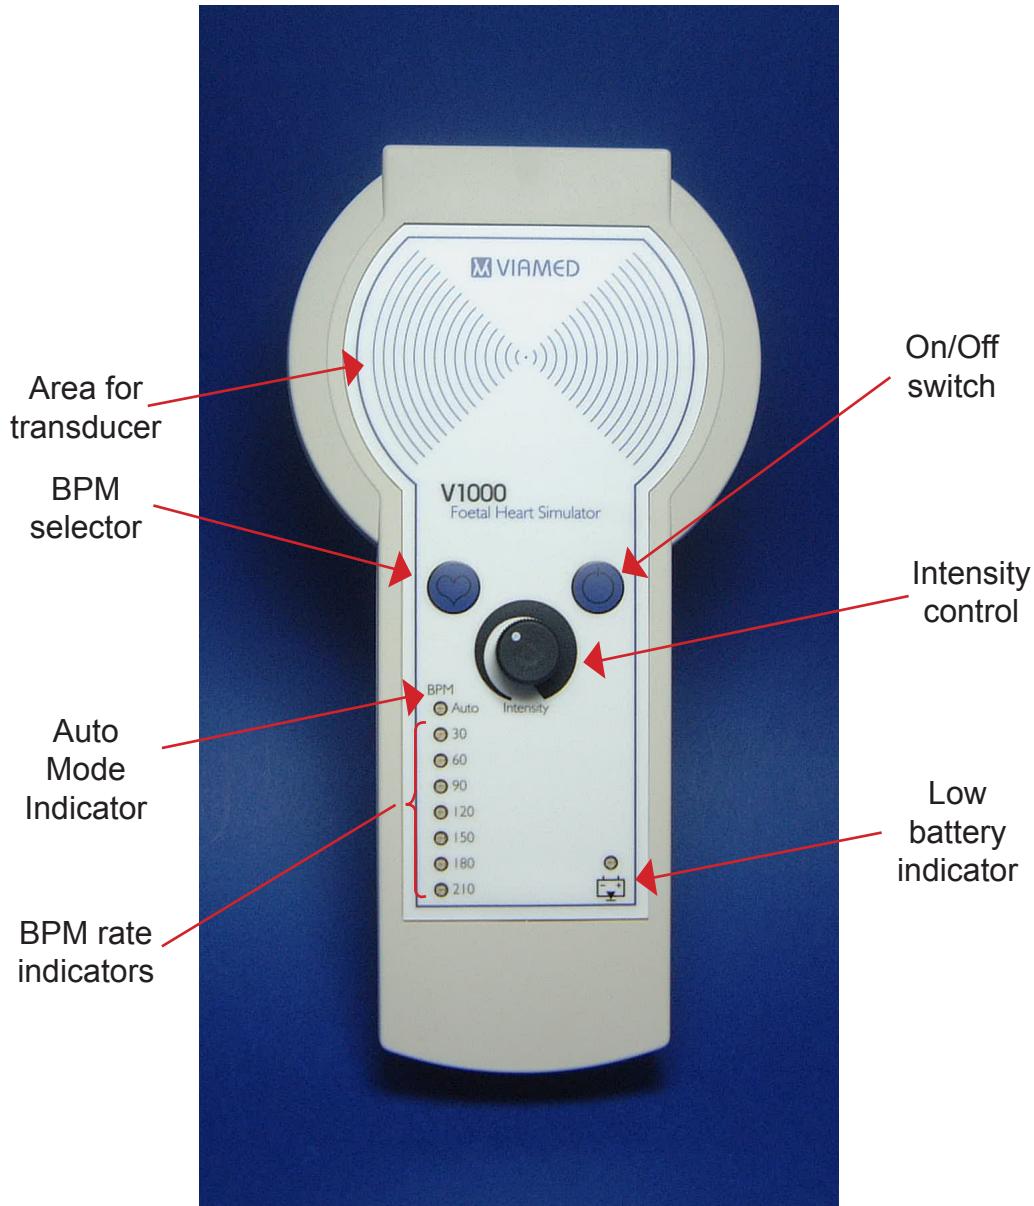

Operating the V1000

The V1000 can simulate at fixed heart rates between 30 BPM and 210 BPM at 30 BPM intervals. It can also run an automatic test routine of 30 seconds at 30 BPM followed by the same duration at 60, 90, 120, 150, 180 & 210 BPM. This test routine is continuous until auto test is deselected or the simulator is switched off.

1. Place ultrasound gel on the centre of the transducer placement markings on the front panel of the V1000.
2. Obtain a good contact between the transducer and the V1000, with the transducer remaining central, using the concentric markings as a guide.
3. Press the On/Off button and ensure that each of the LED indicators illuminates during the self-test routine.
4. When the self-test routine is complete, the 120 BPM indicator begins to flash. If the low battery indicator is illuminated, replace the batteries.
5. Adjust the intensity control until the foetal heart monitor under test begins to respond, then set the intensity control as necessary.
6. Pressing the BPM selector button adjusts the output rate of the V1000, pressing the button whilst at 210 BPM sets the V1000 into the automatic test routine.
7. To switch off the V1000, press the On/Off button. Ensure that all rate indicators extinguish, detach the transducer and remove any residual gel using a damp cloth.

Low Battery Indication

When the V1000 detects that the batteries are nearing depletion, the low battery indicator will begin to flash. The V1000 can still be used, but the user should consider that simulation may cease at any time without further warning.

When the battery voltage reduces to a level where the performance of the V1000 may be compromised, simulation will cease and the low battery indicator will remain illuminated.

When the low battery indicator is constantly illuminated, the batteries must be replaced.

Replacing the Batteries

The V1000 operates using 4 x 1.5V AA/MN1500/LR6 alkaline batteries.

To replace the batteries, remove the battery door on the rear panel, remove the existing batteries and insert new ones, observing the polarity indications inside the battery compartment.

Depleted batteries should be disposed of as per local regulations.

Caution: only use batteries of the type specified.

Note: If the V1000 is to be removed from service or stored, the batteries must be removed.

Cleaning

With reference to the Medical Devices Agency document “Sterilization, disinfection and cleaning of medical equipment: guidance on decontamination from the Microbiology Advisory Committee to Department of Health Medical Devices Agency” (known as the MAC Manual), “Introduction to Part 1 - Table 1: Classification of infection risk associated with the decontamination of medical devices”; the V1000 Foetal Heart Simulator is classified as low risk, due to being “In contact with healthy skin, or not in contact with the patient”.

The recommended decontamination method for low risk items is to clean in accordance with the guidelines in the MAC Manual “Part 2; Cleaning (manual) - non-immersion”.

Protection Rating

The V1000 is manufactured to an ingress protection rating of IP41.

Routine Maintenance

It is recommended that the V1000 be checked at least annually to ensure correct performance.

Perform functionality checks as detailed on the Performance Evaluation Sheet overleaf. There are no user serviceable parts inside: if the device does not meet the specification or if performance is suspect, please return it to Viamed for evaluation or repair.

Note: The output BPM is governed by the firmware and the microcontroller - there is no adjustable calibration control.

The V1000 is a simulator and is to not be used as a calibration device.

Optional Accessories

Part Number	Description
1420000	Wall mount for Foetal Heart Simulator
1420001	Case protector for use with Foetal Heart Simulator, model V1000. Colour: Grey
0013110	Carrying case Colour: Blue

Warranty

Viamed warranty ensures that goods are free from defects of manufacture for a period of one year from the date of shipment from Viamed.

Notes

V1000 Foetal Heart Simulator Performance Evaluation Sheet

Hospital/Organisation:		
Location (department, room no.):		
Engineer (print):		
Service Date:		
Action		
Serial Number:	Pass	Fail
Batteries replaced		
Comments:		
Check for overall signs of damage		
Comments:		
Check Power - Good Green LED		
Comments:		
Check Power - Low Green LED		
Comments:		
Check all LEDs function		
Comments:		
Check BPM Control		
Comments:		
Check BPM 120		
Comments:		
Check BPM 150		
Comments:		
Check BPM 180		
Comments:		
Check BPM 210		
Comments:		
Check BPM Auto		
Comments:		
Check BPM 30 (if applicable)		
Comments:		
Check BPM 60		
Comments:		
Check BPM 90		
Comments:		
Check Intensity Control Functionality		
Comments:		
Additional notes or comments:		

Notes



ISO 13485:2003

Viamed Limited · 15 Station Road · Cross Hills
Keighley · West Yorkshire · BD20 7DT · United Kingdom
Tel: +44 (0)1535 634 542 Fax: +44 (0)1535 635 582
Email: info@viamed.co.uk Website: www.viamed.co.uk

Operator's Manual
V1000 Foetal Simulator
V3 Nov 2014

Specifications Subject to Change

Operator's Manual Part Number: 1490001
V1000 Part Number: 1410000

