

# VIAMED

## Suppliers of Electromedical Equipment

# 2017



Ingleborough Falls, Ingleton

### January

|   |    |   |    |    |    |
|---|----|---|----|----|----|
| M | 30 | 2 | 9  | 16 | 23 |
| T | 31 | 3 | 10 | 17 | 24 |
| W |    | 4 | 11 | 18 | 25 |
| T |    | 5 | 12 | 19 | 25 |
| F |    | 6 | 13 | 20 | 26 |
| S |    | 7 | 14 | 21 | 28 |
| S | 1  | 8 | 15 | 22 | 29 |

### February

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 6  | 13 | 20 | 27 |
| T |   | 7  | 14 | 21 | 28 |
| W | 1 | 8  | 15 | 22 |    |
| T | 2 | 9  | 16 | 23 |    |
| F | 3 | 10 | 17 | 24 |    |
| S | 4 | 11 | 18 | 25 |    |
| S | 5 | 12 | 19 | 26 |    |

### March

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 6  | 13 | 20 | 27 |
| T |   | 7  | 14 | 21 | 28 |
| W | 1 | 8  | 15 | 22 | 29 |
| T | 2 | 9  | 16 | 23 | 30 |
| F | 3 | 10 | 17 | 24 | 31 |
| S | 4 | 11 | 18 | 25 |    |
| S | 5 | 12 | 19 | 26 |    |

### April

|   |   |   |    |    |    |
|---|---|---|----|----|----|
| M |   | 3 | 10 | 17 | 24 |
| T |   | 4 | 11 | 18 | 25 |
| W |   | 5 | 12 | 19 | 26 |
| T |   | 6 | 13 | 20 | 27 |
| F |   | 7 | 14 | 21 | 28 |
| S | 1 | 8 | 15 | 22 | 29 |
| S | 2 | 9 | 16 | 23 | 30 |

### May

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M | 1 | 8  | 15 | 22 | 29 |
| T | 2 | 9  | 16 | 23 | 30 |
| W | 3 | 10 | 17 | 24 | 31 |
| T | 4 | 11 | 18 | 25 |    |
| F | 5 | 12 | 19 | 26 |    |
| S | 6 | 13 | 20 | 27 |    |
| S | 7 | 14 | 21 | 28 |    |

### June

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 5  | 12 | 19 | 26 |
| T |   | 6  | 13 | 20 | 27 |
| W |   | 7  | 14 | 21 | 28 |
| T | 1 | 8  | 15 | 22 | 29 |
| F | 2 | 9  | 16 | 23 | 30 |
| S | 3 | 10 | 17 | 24 |    |
| S | 4 | 11 | 18 | 25 |    |

### July

|   |    |   |    |    |    |
|---|----|---|----|----|----|
| M | 31 | 3 | 10 | 17 | 24 |
| T |    | 4 | 11 | 18 | 25 |
| W |    | 5 | 12 | 19 | 26 |
| T |    | 6 | 13 | 20 | 27 |
| F |    | 7 | 14 | 21 | 28 |
| S | 1  | 8 | 15 | 22 | 29 |
| S | 2  | 9 | 16 | 23 | 30 |

### August

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 7  | 14 | 21 | 28 |
| T | 1 | 8  | 15 | 22 | 29 |
| W | 2 | 9  | 16 | 23 | 30 |
| T | 3 | 10 | 17 | 24 | 31 |
| F | 4 | 11 | 18 | 25 |    |
| S | 5 | 12 | 19 | 26 |    |
| S | 6 | 13 | 20 | 27 |    |

### September

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 4  | 11 | 18 | 25 |
| T |   | 5  | 12 | 19 | 26 |
| W |   | 6  | 13 | 20 | 27 |
| T |   | 7  | 14 | 21 | 28 |
| F | 1 | 8  | 15 | 22 | 29 |
| S | 2 | 9  | 16 | 23 | 30 |
| S | 3 | 10 | 17 | 24 |    |

### October

|   |    |   |    |    |    |
|---|----|---|----|----|----|
| M | 30 | 2 | 9  | 16 | 23 |
| T | 31 | 3 | 10 | 17 | 24 |
| W |    | 4 | 11 | 18 | 25 |
| T |    | 5 | 12 | 19 | 25 |
| F |    | 6 | 13 | 20 | 26 |
| S |    | 7 | 14 | 21 | 28 |
| S | 1  | 8 | 15 | 22 | 29 |

### November

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 6  | 13 | 20 | 27 |
| T |   | 7  | 14 | 21 | 28 |
| W | 1 | 8  | 15 | 22 | 29 |
| T | 2 | 9  | 16 | 23 | 30 |
| F | 3 | 10 | 17 | 24 |    |
| S | 4 | 11 | 18 | 25 |    |
| S | 5 | 12 | 19 | 26 |    |

### December

|   |   |    |    |    |    |
|---|---|----|----|----|----|
| M |   | 4  | 11 | 18 | 25 |
| T |   | 5  | 12 | 19 | 26 |
| W |   | 6  | 13 | 20 | 27 |
| T |   | 7  | 14 | 21 | 28 |
| F | 1 | 8  | 15 | 22 | 29 |
| S | 2 | 9  | 16 | 23 | 30 |
| S | 3 | 10 | 17 | 24 | 31 |



# VIAMED

15 Station Road · Cross Hills · Keighley · West Yorkshire · BD20 7DT · UK  
Tel: +44 (0)1535 634 542 · Fax: +44 (0)1535 635 582  
info@viamed.co.uk · www.viamed.co.uk





# VM-2500 Series Capnographs

To address the growing emphasis on the use of Capnography during resuscitation and intubation,

**Viamed offer the VM-2500 range of high performance Capnographs**


Available as Mainstream and Sidestream units; along with a range of VersaStream one-piece sampling lines (sidestream only)




**Full scale accuracy within 10 seconds**



Nasal Sampling Line

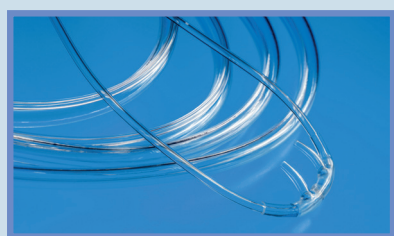

Nasal Cannula

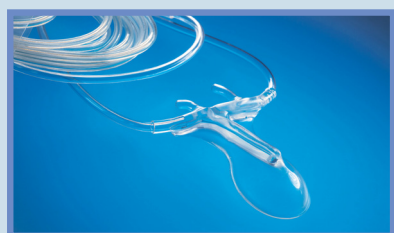

Nasal/Oral Cannula



Airway Adapter Sampling Line


## VersaStream® CO<sub>2</sub> Sampling Lines

**The alternative to Nafion® & Water Traps**

Innovative solutions for sidestream monitoring for use with a range of manufacturers' capnographs including Philips, GE, Respirationics, Dräger and Viamed...

A one-piece sampling solution with integrated bacterial filter with active & complete removal of moisture and water, providing increased performance and reducing cost.

**To find out more visit our Cross Reference**  
**[www.viamed.co.uk/linesxref](http://www.viamed.co.uk/linesxref)**

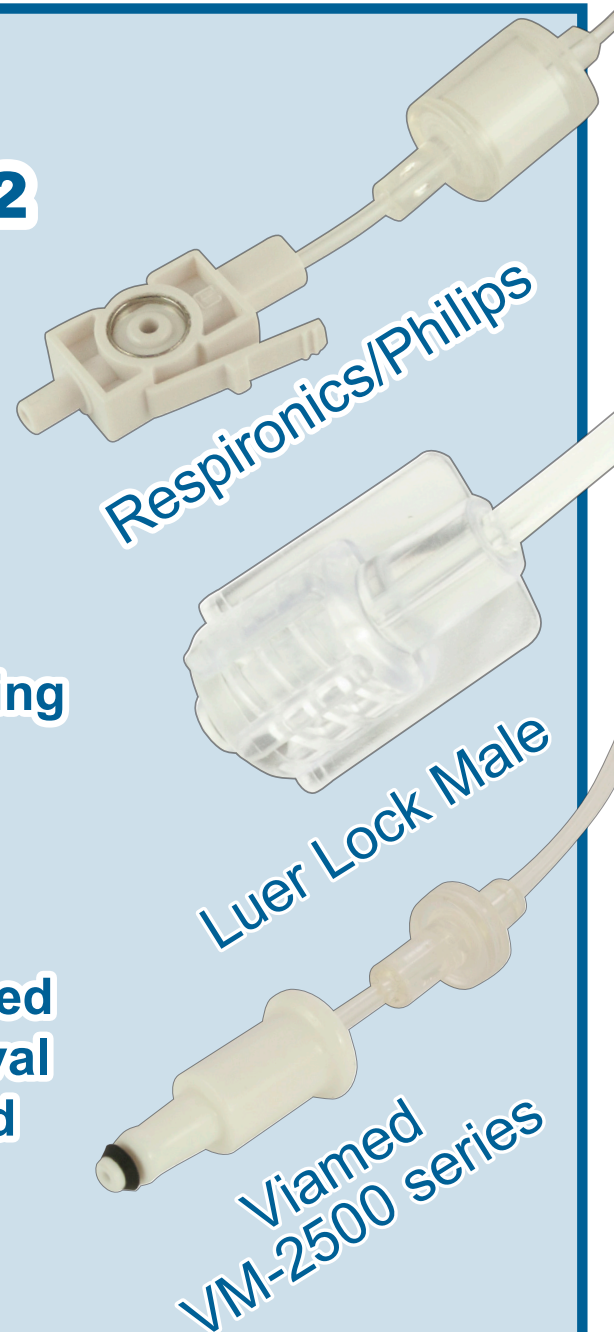

**VIAMED**

**Tel: 01535 634 542**

Specifications Subject to Change  
Part Number: 0196000

