




# MaxBlend Lite Compatibility

This leaflet details the characteristics required of oxygen/air blenders to be compatible with the **MaxBlend Lite**.

All medical oxygen air blenders have similar performance requirements in order to comply with international standards (ISO11195 Gas mixers for medical use - Stand-alone gas mixers). However, the physical shape of the blender varies from model to model.

The following requirements detail the blender requirements necessary for compatibility with the **MaxBlend Lite**. If you are unsure if your blender meets these requirements, please contact Viamed for assistance.

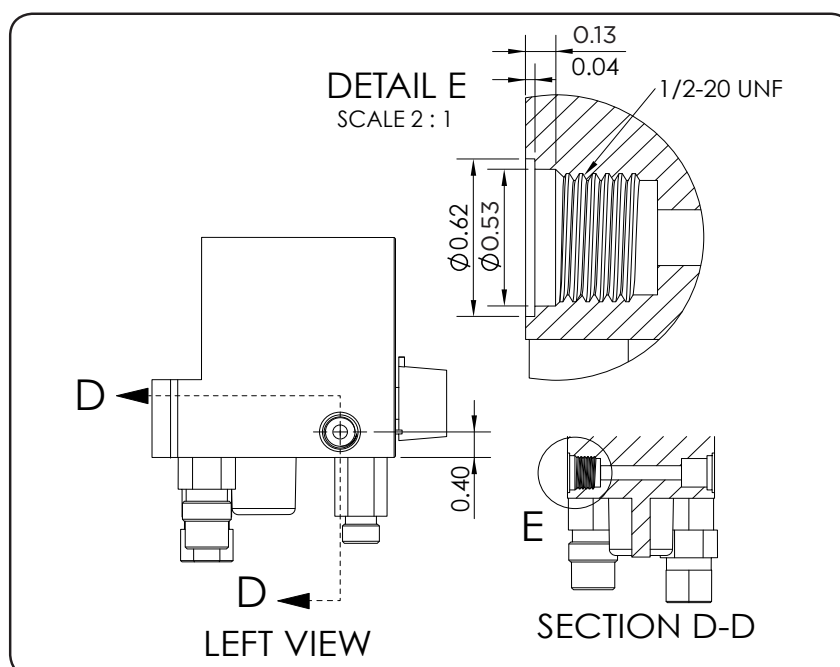

**VIAMED**

**Viamed Limited** · 15 Station Road · Cross Hills  
 Keighley · West Yorkshire · BD20 7DT · United Kingdom  
 Tel: +44 (0)1535 634 542 Fax: +44 (0)1535 635 582  
 Email: [info@viamed.co.uk](mailto:info@viamed.co.uk) Website: [www.viamed.co.uk](http://www.viamed.co.uk)